

ANDROFLOR®:

a brief guide to results interpretation

ANDROFLOR®:

a brief guide to results interpretation

- Androflor® is a comprehensive real-time PCR-based assay for the assessment of the state of the male urogenital tract microbiota and detection of obligate pathogens — causative agents of sexually transmitted infections (STIs).
- The Androflor® test has no analogues in the world.
- Androflor® allows rapid* quantitative determination of normal and opportunistic microbiota components, including anaerobic microorganisms that are difficult to culture, as well as detection of obligate pathogens *Chlamydia trachomatis*, *Mycoplasma genitalium*, *Neisseria gonorrhoeae* and *Trichomonas vaginalis*.

This guide discusses the options for choosing a test from the Androflor® product line, the specifics of biomaterial sampling and interpretation of the results.

* hands-on time: from 3 hours

CONTENT

CHOOSING A TEST FROM THE ANDROFLOR® PRODUCT LINE	3
BIOMATERIAL SAMPLING	7
Specifics of biomaterial sampling for Androflor® assay	7
Biomaterial storage and transportation conditions	10
Information for laboratories on ejaculate testing	10
ANALYSIS OF RESULTS	11
Guidance note for the result form interpretation	12
Control indicators of the biomaterial sampling quality	14
Microbiome composition of the male urogenital tract	15
Obligate pathogens	16
Scheme of the results interpretation	16
EXAMPLES OF RESULTS FORM	18
1. The bacterial microbiome composition is normal	18
What is considered as a norm for the male urogenital tract?	18
If TBM is low, should the collection of biomaterial be repeated?	21
Why TBM might be missing?	22
Why is there no color indication on the results form?	25
2. The bacterial microbiome composition is abnormal	26
Absolute predominance of one of the groups of normal microbiota (microflora)	26
The balance of normal and opportunistic microbiota is moderately disturbed	27
The balance of normal and opportunistic microbiota is severely disturbed	31
Significant decrease/absence of normal microbiota is not proportional to the absence/slight increase of opportunistic microbiota	34
STIs DNA is detected (obligate pathogens are present)	36
3. Cases when no conclusion is issued	37
Insufficient amount of biomaterial: TBM and Human DNA are both not detected or below threshold	37
Exceeding the threshold values of transient microbiota	38
Will obligate pathogens be detected, if human DNA and TBM are not detected?	40

CHOOSING A TEST FROM THE ANDROFLOR® PRODUCT LINE

The Androflor® line includes the Androflor® and Androflor® Screen assays. Both assays are used to detect the obligate pathogens *Chlamydia trachomatis*, *Mycoplasma genitalium*, *Neisseria gonorrhoeae*, *Trichomonas vaginalis* and to quantify components of the normal and opportunistic microbiota (bacteria and yeast fungi of the genus *Candida*).

The main difference between the assays is the profile of the determined opportunistic microorganisms (OM) and, therefore, the indications for prescribing the tests.

Androflor® Screen is a shortened version of the assay, which is intended for screening and differential diagnosis of acute forms of urogenital tract diseases.

Androflor® is a detailed assay for accessing of microbiome structure, which detects a wide range of opportunistic microorganisms. This assay is recommended to prescribe for patients with chronic forms of diseases or complaints of ineffective treatment. Also, it can help to determine the possible impact of infections on reproductive function while preparing for IVF.

Androflor® Screen	Androflor®
<i>Staphylococcus spp.</i> <i>Streptococcus spp.</i> <i>Corynebacterium spp.</i>	<i>Staphylococcus spp.</i> <i>Streptococcus spp.</i> <i>Corynebacterium spp.</i>
<i>Lactobacillus spp.</i>	<i>Lactobacillus spp.</i>
<i>Gardnerella vaginalis</i> <i>Ureaplasma urealyticum</i> <i>Ureaplasma parvum</i> <i>Mycoplasma hominis</i> <i>Enterobacteriaceae / Enterococcus spp.</i> <i>Candida spp.</i>	<i>Gardnerella vaginalis</i> <i>Megasphaera spp. / Veillonella spp. / Dialister spp.</i> <i>Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.</i> <i>Ureaplasma urealyticum</i> <i>Ureaplasma parvum</i> <i>Mycoplasma hominis</i> <i>Atopobium cluster</i> <i>Bacteroides spp. / Porphyromonas spp. / Prevotella spp.</i> <i>Anaerococcus spp.</i> <i>Peptostreptococcus spp. / Parvimonas spp.</i> <i>Eubacterium spp.</i> <i>Haemophilus spp.</i> <i>Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.</i> <i>Enterobacteriaceae spp. / Enterococcus spp.</i> <i>Candida spp.</i>
<i>Mycoplasma genitalium</i> <i>Trichomonas vaginalis</i> <i>Neisseria gonorrhoeae</i> <i>Chlamydia trachomatis</i>	<i>Mycoplasma genitalium</i> <i>Trichomonas vaginalis</i> <i>Neisseria gonorrhoeae</i> <i>Chlamydia trachomatis</i>

Depending on the specifics of the clinical situation and the objectives of the examination, other PCR tests may be prescribed in addition to the Androflor® test at the discretion of the physician, for example, detection of *HSV1/HSV2/CMV* herpesviruses (HSV1, HSV2, CMV Multiplex) or human papillomaviruses (HPV-Quant-21).

NB! Please consult with your medical diagnostic laboratory on the possibility of conducting multiple PCR tests using a single biomaterial sample.

For differential diagnostics of chronic recurrent diseases in a couple and searching for possible causes of infertility, it is advisable to carry out a comprehensive quantitative assessment of reproductive tract microbiota for both partners using Androflor® and Femoflor® line assays.


Example of a couple examination using the Androflor® and Femoflor®16 assays

A male patient presented with complains on pain in the area of the glans of the penis and redness of the foreskin. His female partner had itching and genital irritation after sexual intercourse.

A sample of urethral scrape obtained from the male was examined using the Androflor® test system. A vaginal scrape sample from the female was examined using the Femoflor®16 test system.


Urogenital microbiome composition test Androflor®

Date
 Number of tube
 Patient name
 Sex
 Age
 Organization
 Clinician name
 Comments
 Sample ID:



Information about laboratory

№	Test title	Result	
		Quantitative	Relative Lg(X/TBM)
	Human DNA	10 ^{5.7}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{4.5}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{3.1}	-1,4 [3-5%]
	Commensals, sum	10 ^{3.1}	-1,4 [3-5%] ■
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	10 ^{3.6}	-0,9 [11-14%] ■
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	10 ^{3.6}	-0,9 [11-14%] ■
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	10 ^{4.3}	-0,2 [54-73%] ■
14	Anaerococcus spp.	10 ^{3.8}	-0,7 [17-23%] ■
15	Peptostreptococcus spp. / Parvimonas spp.	10 ^{3.6}	-1,1 [7-9%] ■
16	Eubacterium spp.	10 ^{4.3}	-0,2 [54-73%] ■
	Opportunistic anaerobes, sum	10 ^{4.7}	0,2 [85-100%] ■
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{3.3}	-1,2 [5-7%] ■
Yeast-like fungi			
20	Candida spp. *	10 ^{3.2}	■
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

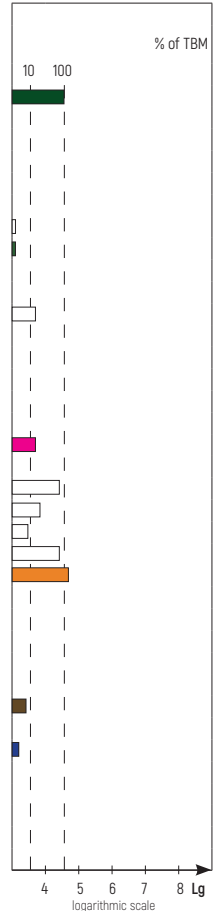

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:


STIs DNA is not detected.

DETECTED: Candida spp.

The bacterial microbiome composition is abnormal: opportunistic bacteria are detected.

Urogenital microbiome composition test Femoflor®16


Date
 Number of tube
 Patient name
 Sex
 Age
 Organization
 Clinician name
 Comments



Information about laboratory

Sample ID:

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Sample intake control	10 ^{6.8}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{7.7}	<input type="checkbox"/>
NORMAL MICROFLORA			
2	Lactobacillus spp.	10 ^{7.3}	-0,3 (39-53%) ■
FACULTATIVE ANAEROBIC MICROORGANISMS			
3	Enterobacteriaceae	not detected	<input type="checkbox"/>
4	Streptococcus spp.	not detected	<input type="checkbox"/>
5	Staphylococcus spp.	10 ^{3.3}	-4,3 (<0,1%) <input type="checkbox"/>
OBLIGATE ANAEROBIC MICROORGANISMS			
6	Gardnerella vaginalis + Prevotella bivia + Porphyromonas spp.	10 ^{7.2}	-0,4 (31-42%) ■
7	Eubacterium spp.	10 ^{6.8}	-0,8 (12-17%) ■
8	Sneathia spp. + Leptotrichia spp. + Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Megasphaera spp. + Veillonella spp. + Dialister spp.	10 ^{6.0}	-1,6 (2,0-2,7%) ■
10	Lachnobacterium spp. + Clostridium spp.	not detected	<input type="checkbox"/>
11	Mobiluncus spp. + Corynebacterium spp.	not detected	<input type="checkbox"/>
12	Peptostreptococcus spp.	not detected	<input type="checkbox"/>
13	Atopobium vaginae	not detected	<input type="checkbox"/>
YEAST-LIKE FUNGI			
14	Candida spp. *	10 ^{5.6}	■
MYCOPLASMAS			
15	Mycoplasma hominis *	not detected	<input type="checkbox"/>
16	Ureaplasma (urealyticum + parvum) *	not detected	<input type="checkbox"/>
PATHOGENIC MICROORGANISMS			
17	Mycoplasma genitalium **	not detected	<input type="checkbox"/>

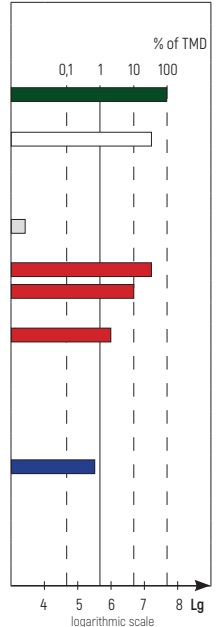

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

MODERATE ANAEROBIC DYSBIOSIS

Pathogenic microorganisms were not detected in both partners.

Both patients had a decrease in the amount of normal microbiota with an increase in the number of anaerobic opportunistic microorganisms. In the female patient *Candida spp.* were present in clinically significant amounts.

Based on the results of Androflor® and Femoflor®16, effective etiotropic therapy was prescribed and carried out in both partners.

BIOMATERIAL SAMPLING

To obtain correct real-time PCR results, the pre-analytical stage is of great importance: preparation of a patient for the study, selection of biomaterial type and quality of biomaterial collection, conditions of sample storage and transportation to the laboratory.

The choice of biomaterial for Androflor® and Androflor® Screen assays depends on the diagnostic goals (Table 1).

It is important to take into account **the special rules of preparation for the study:**

- **Sexual abstinence or use of barrier contraception for 3 days** before the study is recommended to minimize the risk of contamination of the biomaterial with the microbiota of a sexual partner.
- The use of **antiseptics**, including antibacterial soaps, **should be avoided**.

Prescription of the Androflor® study while taking antibiotics is possible (for example, to monitor therapy), but it should be taken into account that antibiotic therapy can affect the results.

Specifics of biomaterial sampling for Androflor® assay

The study of microorganisms' DNA by real-time PCR is a direct laboratory method, so the biomaterial should be obtained from localizations as close as possible to the suspected focus of the infectious process.

Table 1: recommended biomaterial and technique of its sampling for study by Androflor® assay

BIOMATERIAL	PURPOSE OF DIAGNOSTICS	SPECIFICS OF PREPARATION	RULES OF SAMPLING
Epithelial scrapes from the glans of the penis (penis balanus), foreskin, preputial sac, urethra	Identification of etiology of acute and chronic infectious-inflammatory processes of lower urogenital tract (urethritis, balanoposthitis)	<p>A patient is recommended to avoid urinating within 1.5-2 hours prior to sampling procedure.</p> <p>It is important to take the maximum amount of epithelial cells and the minimum amount of mucus</p>	<p>The scraping is performed with a sterile, disposable urogenital swab. After biomaterial taking, the swab should be put into a 1.5 ml plastic tube with transport medium. Rinse the swab thoroughly, then remove the swab from solution, press it to the wall of tube and squeeze the rest of the liquid. A swab shouldn't be broken off or left in the tube.</p> <p>Features of the urethral sampling The external urethral orifice must be treated with a swab moistened with sterile physiological saline solution just prior to the sampling procedure. In the case of purulent discharge, the sample must be taken 15-20 minutes after urinating. Carefully insert the swab into the urethra to a depth up to 5 cm, then carefully rotate to the external urethral orifice</p>
Urine	Identification of the etiology of acute inflammatory processes (STIs only) associated with pronounced pain on insertion of a swab into the urethra	In the absence of acute inflammation, the number of human cells in a sample may be very low and the Human DNA indicator value can be below the threshold	The first portion of morning urine in the minimum possible amount of 10–15 ml is collected into a special dry sterile container with a volume of up to 60 ml, equipped with a hermetically screw-cap
	Diagnosis of urinary infections	It is more preferable to prescribe the BacScreen OM assay, as it includes microorganisms associated with urinary tract infections	
Ejaculate	Diagnosis of epididymitis, prostatitis, STIs with asymptomatic course, male infertility	Ejaculate should not be obtained by interrupted sexual intercourse (as an admixture of transient microbiota is possible) or from a condom (as lubricant components inhibit PCR)	<p>Ejaculate is collected by a patient only by manual masturbation into a sterile container of up to 60 ml and can be obtained in the laboratory or at home.</p> <p>The collected biomaterial should be stored in the refrigerator for no more than 24 hours or frozen</p>

BIOMATERIAL	PURPOSE OF DIAGNOSTICS	SPECIFICS OF PREPARATION	RULES OF SAMPLING
Prostatic fluid	Diagnosis of epididymitis, prostatitis, STIs with asymptomatic course, male infertility	Sexual abstinence is recommended for 3 days before the examination. If acute prostatitis is suspected, prostate massage is strictly prohibited!	The glans of the penis (penis balanus) is treated with a sterile cotton swab moistened with saline solution. Prostatic fluid is collected after preliminary prostate massage through the rectum. The massage is performed by a doctor through a vigorous pressing movement from the base to the top of the gland. The released prostatic fluid in the form of a free-flowing drop (0.5-1.0 ml) is collected in a disposable sterile dry tube with a volume of 2 ml or in a container with a volume of up to 60 ml
Residual urine after prostate massage	Diagnosis of epididymitis, prostatitis, STIs with asymptomatic course, male infertility	Sexual abstinence is recommended for 3 days before the examination. If acute prostatitis is suspected, prostate massage is strictly prohibited!	A patient should urinate in a toilet, leaving some urine in the bladder. Before collecting urine, the glans of the penis is treated with a sterile cotton swab moistened with saline solution. After this, the patient is subjected to prostate massage for 1-3 minutes. The intensity of massage depends on the density of the prostate: if the prostate is soft, gentle pressure is applied, if the prostate is dense, the intensity of pressure should be increased. After prostate massage, the patient collects the first 10-15 ml of urine into a sterile plastic container with a volume of up to 60 ml
Biopsy samples from prostatic tissues	Diagnosis of epididymitis, prostatitis, STIs with asymptomatic course, male infertility		Biopsy sample is placed in a sterile tube with sterile saline solution or water (in volume no more than 0.5 ml), or in an empty sterile tube

Biomaterial storage and transportation conditions



Biomaterial for PCR examination can be stored at a temperature from 2 °C to 8 °C for 24 hours, so the sample should be transferred to the laboratory within a day or else frozen.

Frozen material can be stored at temperatures from -18 °C to -22 °C for no more than one month.

INFORMATION FOR LABORATORIES ON EJACULATE TESTING

When extracting DNA from ejaculate, it is recommended to use 100 µl of sample. For DNA extraction from ejaculate it is recommended to use the PREP-MB MAX kit. It is also possible to perform DNA extraction using PREP-NA PLUS and PREP-GS PLUS kits.

ANALYSIS OF RESULTS



The Androflor® assay uses genome-equivalent (GE)/sample as a unit of measurement. The GE is the amount of genetic material corresponding to one genome of a microorganism. This unit of measurement of the PCR method is similar to the CFU in a microbiological culture. If it is necessary to establish the ratios of microorganisms in the microbiota, relative values, or proportions, are used.


In the Androflor® assay line, indicator values are represented in two formats: absolute and relative.

- Absolute values are expressed in genome-equivalents (GE/sample) and are proportional to the urogenital biotope microbial load for each detected microorganism.
- Relative values are expressed in % and represent the proportion of each taxon in the total bacterial mass. Values are presented as ranges to account for method inaccuracy. PCR is performed independently for each of the microorganisms, including the TBM (total bacterial mass), so the sum of the relative values will not be necessarily equal to 100%, thus it is not correct to sum the relative values.

Guidance note for the result form interpretation

The diagrams below show the handouts for interpreting the Androflor® and Androflor®Screen result forms.

Androflor®

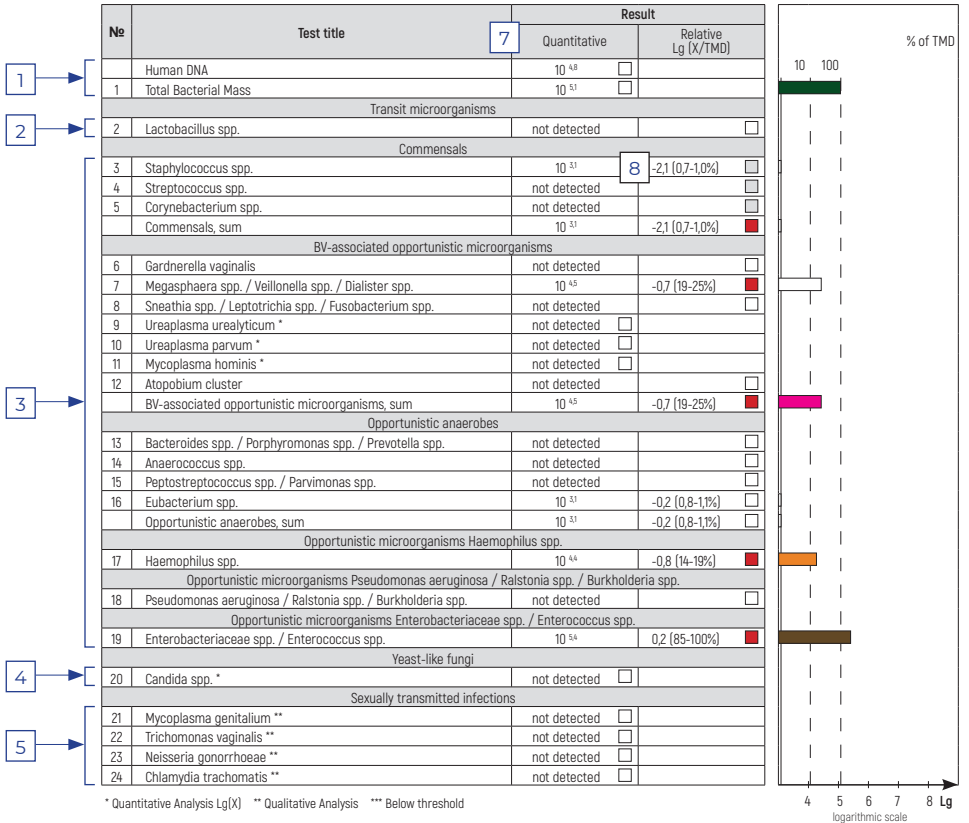

Conclusion:

STIs DNA is not detected.

Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: the balance of normal and opportunistic microflora is severely disturbed (with Enterobacteriaceae spp. / Enterococcus spp. predominance).

Androflor® Screen

№	Test title	Result	
		Quantitative	Relative Lg (X/TBM)
1	Human DNA	10 ^{4.9}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{8.8}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	10 ^{5.5}	-1.2 (5-7%) <input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	10 ^{5.5}	-1.2 (5-7%) <input type="checkbox"/>
5	Corynebacterium spp.	10 ^{5.8}	-0.1 (85-100%) <input type="checkbox"/>
	Commensals, sum	10 ^{5.8}	-0.1 (85-100%) <input type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
8	Ureaplasma parvum *	not detected	<input type="checkbox"/>
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{5.1}	-1.6 (2.1-2.9%) <input type="checkbox"/>
Yeast-like fungi			
11	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.
Candida spp. is below threshold.
The bacterial microbiome composition is normal.

- 1 **Estimation of biomaterial quantity**
 - The number of human cells
 - The number of bacteria
- 2 **Assessment of transient microbiota**
 - Marker of admixture of female urogenital microbiota
 - It is called «Transit microorganisms» in the report form
- 3 **Assessment of microbiota structure**
 - Amount of normal microbiota
 - Number of opportunistic microorganisms
- 4 **Assessment of yeast fungi**
- 5 **Assessment of obligate pathogens (STIs)**
- 6 **Laboratory conclusion**
- 7 **Absolute values** – the number of genome equivalents/sample
Relative values – the proportion of the microorganisms group in TMD or TBM
- 8 **Percentage of a microorganism in a sample**, taking into account the measurement error

- The value in the «Relative Lg» column turns negative if the microorganism's DNA amount is less than total bacterial mass.
- Summing the percentages in the «Relative Lg» column does not give an informative result. The sum of the percentages may not be equal to 100% due to method specificities.

Control indicators of the biomaterial sampling quality

Parameter «Human DNA» shows the amount of human genomic DNA in a sample. Human DNA value can vary in different types of biomaterial, for example, in urine it can be very low (may be as a norm or in case of chronic forms of prostatitis) or high (in acute urethritis).

Total Bacterial Mass (TBM) is the total number of bacteria in a sample. This indicator is used to assess the structure of the microbiome by determining the proportion of specific microorganisms and groups of microorganisms in the number of all bacteria.

It should be taken into account that *Candida spp.* (yeast fungi) and *Trichomonas vaginalis* (protozoan, a unicellular parasite) are not bacteria and thus are not included in TBM.

Total Microorganisms Detected (TMD) is a mathematically calculated parameter that is used to estimate the ratios of microorganism groups in a sample.

- **NB!** If TBM and Human DNA indicators are both below the threshold values in the results, no further analysis of the microbiome composition is performed, as there is no verification of correct biomaterial sampling. In this case the results of the assay can be interpreted only by an attending physician, based on the specifics of a clinical situation. At the same time, correct results will be obtained for the detection of obligate pathogens and *Candida* fungi, which will be reported in the conclusion. In these cases, a repeated biomaterial sampling and retesting can be recommended, with the requirement of compliance with the rules of patient preparation for the study.
- If **at least one** of TBM and Human DNA indicators is above the threshold, the automatic analysis of the microbiome composition is performed.

Examples of result forms interpretation are provided on page 18.

Transit microorganisms (*Lactobacillus spp.*)

The presence of *Lactobacillus spp.* and their proportion in TBM are assessed as a marker of presence of a female partner's microbiota in a male patient's urogenital tract.

Lactobacillus spp. can be detected within several days after an unprotected sexual intercourse when analyzing biomaterial of a male patient using Androflor® and Androflor® Screen test systems.

If a relative amount of *Lactobacillus spp.* in a sample is above the threshold value (10% of TBM), the microbiome composition is not analyzed in the Androflor® tests. The reason is that actual composition of male microbiota may be distorted by presence of significant amounts of female microbiota. This factor is especially important in the diagnosis of chronic diseases of urogenital tract. The automatic conclusion for these cases issues an indication of improper patient preparation for the examination and recommends to repeat biomaterial sampling under the condition of protected sexual contacts or sexual abstinence within 3 days.

It is worth noting that there are patients in clinical practice who have a significant amount of *Lactobacillus spp.* in their ejaculate, even if preparation for the examination is carried out properly. The presence of *Lactobacillus spp.* in ejaculate may serve as an additional marker of hormonal disturbance in men, even in those with normal spermogram indicators [1].

It should also be taken into account that detected opportunistic microorganisms, including those associated with bacterial vaginosis, may be a part of a female partner's microbiota and cause acute inflammation of the lower urogenital tract in a man.

Microbiome composition of the male urogenital tract

Normal microbiota (commensals)

Normal microbiota of male urogenital tract is represented by bacteria of the genera *Staphylococcus*, *Streptococcus* and *Corynebacterium*. Normally all the three groups should together constitute a major part of TBM. At the same time, predominance of only one group in simultaneously with significant TBM value is not considered as a variant of norm and indicates a disturbance in the bacterial microbiome composition.

Opportunistic microorganisms (OM)

Opportunistic microorganisms can be categorized into several groups:

- Opportunistic microorganisms associated with bacterial vaginosis (BV)
- Opportunistic anaerobes
- OM *Haemophilus spp.*
- OM *Pseudomonas aeruginosa* / *Ralstonia spp.* / *Burkholderia spp.*
- OM *Enterobacteriaceae spp.* / *Enterococcus spp.*

BV-associated opportunistic microorganisms include some obligate anaerobes and genital mycoplasmas, which are common causative agents of bacterial vaginosis in women, and may cause inflammation in the male urogenital tract as well.

[1] Pochernikov DG, Postovoytenko NT, Getman VV, Galkina IS. Diagnostic significance of *Lactobacillus spp.* identification in ejaculate. Bulletin of RSMU, 2020, 3. DOI: 10.24075/vrgmu.2020.039

The results for opportunistic mycoplasmas (*Ureaplasma urealyticum*, *Ureaplasma parvum*, *Mycoplasma hominis*) and yeast fungi of the genus *Candida* are given only in absolute values in the result form. Relative assessment is not carried out, as their clinical significance is determined by their quantity in a sample, regardless of their proportion in TBM.

For other representatives of opportunistic microorganisms, the proportion in TBM is determined.

- ! NB! *Candida spp.* yeast fungi are not considered as a part of bacterial microbiome composition (that is, the indicator «*Candida spp.*» is not a component of TBM).

Obligate pathogens

Obligate pathogens (*Mycoplasma genitalium*, *Trichomonas vaginalis*, *Neisseria gonorrhoeae*, *Chlamydia trachomatis*) are causative agents of STIs. Their presence in any quantity is considered a pathology, so the results of their detection are reported in a qualitative format. The results of obligate pathogens detection do not depend on other test values, including control indicators (TBM, Human DNA, transit microorganisms).

Scheme of the result form interpretation



Human DNA is the amount of human DNA (cells) in a biomaterial sample. This indicator is determined by PCR results.




TBM is the total number of all bacteria in a biomaterial sample. This indicator is determined by PCR results.




TMD is the sum of the quantities of all microorganisms specifically detected by the Androflor® or Androflor® Screen test. This indicator is calculated mathematically by the software. It may not be equal to the TBM.

The 1st step — assessment of the obligate pathogens and *Candida spp.* presence

These microorganisms are reported in the conclusion even in case of insufficient amount of biomaterial

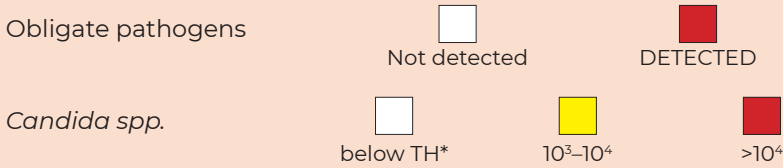

The 2nd step — control of biomaterial compliance with the analysis requirements

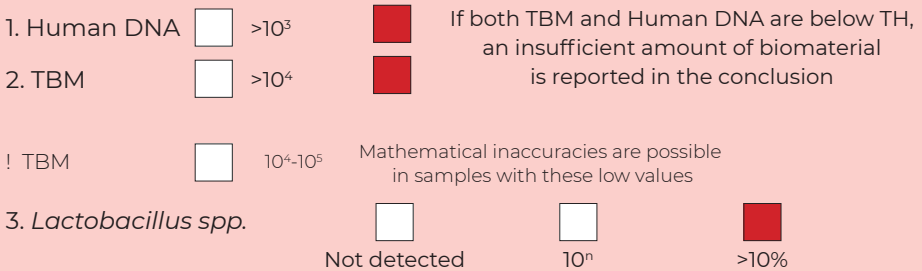

The 3rd step — assessment of the balance between normal and opportunistic microbiota

The bacterial microbiome composition is normal	✓	Predominance of normal microbiota
	✓	Normal microbiota is represented by 2 or more genera at TBM $>10^5$
	✓	Normal microbiota is represented by a single genus at TBM $<10^5$
The bacterial microbiome composition is abnormal	✓	Low bacterial load in a sample
	✗	The proportion of normal microbiota is decreased
	✗	Predominance of opportunistic microorganisms
	✗	Normal microbiota is represented by a single genus at TBM $>10^5$

The 4th step — generation of an automatic conclusion

- Presence of obligate pathogens
- Presence of *Candida spp.*
- Assessment of the bacterial microbiome structure with the determination of a predominant group of microorganisms

* below TH (below threshold value) – below the level of significance

EXAMPLES OF RESULTS FORM

1. The bacterial microbiome composition is normal

WHAT IS CONSIDERED AS A NORM FOR THE MALE UROGENITAL TRACT?

The dominance of normal microbiota (commensals) in a sample in the absence of pathogens is considered as a norm. A minor content of opportunistic microorganisms is acceptable.


At the same time, normal microbiota should be represented by more than one group of microorganisms (Example 1). If only one representative of the normal microbiota is observed in a sample with a high level of bacterial load (TBM), it is concluded that the microbiome composition is disturbed (Example 7).

Specifics of norm interpretation in case of low bacterial load in the sample (TBM <10⁵)

- In some cases, when human DNA content is sufficient for analysis (at «Human DNA» value above threshold values), no microorganisms are detected in a sample. This is especially common in ejaculate examination. These results are considered as a norm (Examples 3-5).
 - In case of low TBM, presence of only one group of normal microbiota is also interpreted as a variant of norm (Example 6).
- ! The presence of *Candida spp.* is reported separately and is not considered as part of the bacterial microbiome composition. Clinical interpretation of the result of *Candida spp.* detection is made by an attending physician (Example 2).

Example 1. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	10 ^{4.6}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{4.8}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	10 ^{3.1}	-1,5 (3-4%) <input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	10 ^{4.8}	0,2 (85-100%)
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{4.5}	-0,1 (68-91%)
	Commensals, sum	10 ^{5.0}	0,4 (85-100%) <input checked="" type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>
14	Anaerococcus spp.	not detected	<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	10 ^{3.4}	-1,2 (5-7%) <input type="checkbox"/>
	Opportunistic anaerobes, sum	10 ^{3.4}	-1,2 (5-7%) <input type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
20	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

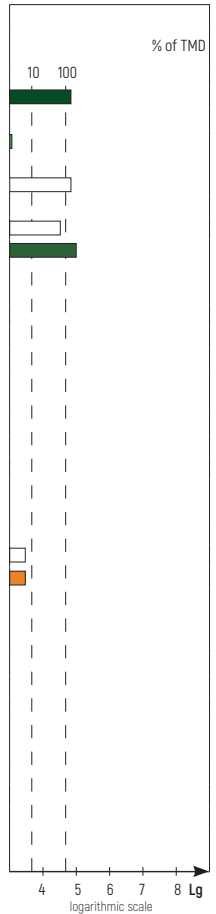

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:


STIs DNA is not detected.

Candida spp. is below threshold.

The bacterial microbiome composition is normal.

Example 2. Androflor® Screen assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TBM)
	Human DNA	10 ^{5.0}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{4.8}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	10 ^{4.7}	-0,1 (68-91%)
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{3.2}	-1,6 (2,1-2,9%)
	Commensals, sum	10 ^{4.7}	-0,1 (70-94%)
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
8	Ureaplasma parvum *	below TH ***	<input type="checkbox"/>
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
11	Candida spp. *	10 ^{3.6}	<input checked="" type="checkbox"/>
Sexually transmitted infections			
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

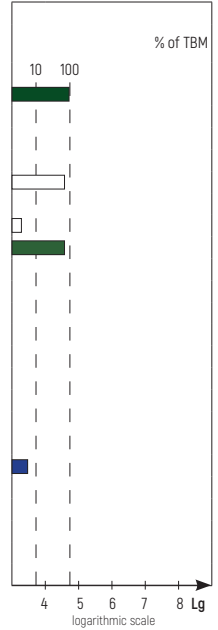

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

DETECTED: Candida spp.

The bacterial microbiome composition is normal.

IF TBM IS LOW, SHOULD THE COLLECTION OF BIOMATERIAL BE REPEATED?

Low TBM value on passing the biomaterial sampling control (with Human DNA value above the threshold) is interpreted as a variant of norm (Example 3). Repeated biomaterial sampling is not required.

Example 3. Androflor® assay

№	Test title	Result		% of TBM
		Quantitative	Relative Lg [X/TBM]	
	Human DNA	10 ^{5.4}	<input type="checkbox"/>	
1	Total Bacterial Mass	10 ^{3.3}	<input type="checkbox"/>	
Transit microorganisms				
2	Lactobacillus spp.	not detected	<input type="checkbox"/>	
Commensals				
3	Staphylococcus spp.	not detected		
4	Streptococcus spp.	not detected		
5	Corynebacterium spp.	not detected		
	Commensals, sum	not detected	<input type="checkbox"/>	
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>	
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>	
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>	
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>	
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>	
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>	
12	Atopobium cluster	not detected	<input type="checkbox"/>	
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>	
Opportunistic anaerobes				
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>	
14	Anaerococcus spp.	not detected	<input type="checkbox"/>	
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>	
16	Eubacterium spp.	not detected	<input type="checkbox"/>	
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Haemophilus spp.				
17	Haemophilus spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.				
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>	
Yeast-like fungi				
20	Candida spp. *	below TH ***	<input type="checkbox"/>	
Sexually transmitted infections				
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>	
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>	
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>	
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>	

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

4 5 6 7 8 Lg
logarithmic scale

Conclusion:

STIs DNA is not detected.

Candida spp. is below threshold.

The bacterial microbiome composition is normal.


WHY TBM MIGHT BE MISSING?

Absence of TBM with presence of Human DNA is not an indication of an insufficient amount of biomaterial. This may be a variant of norm for some types of biomaterial.

In examples 4 and 5, the tested biomaterial was ejaculate. The Androflor® results detected Human DNA, but no TBM or any bacteria (*Candida spp.* are yeast fungi and are not included in TBM). In these cases, biomaterial was taken correctly (as Human DNA indicator is above the threshold), however, ejaculate is characterized by low bacterial load. This represents a variant of norm.

Example 4. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	10 ^{4.5}	<input type="checkbox"/>
1	Total Bacterial Mass	not detected	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	not detected	
	Commensals, sum	not detected	<input type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>
14	Anaerococcus spp.	not detected	<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	not detected	<input type="checkbox"/>
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
20	Candida spp. *	10 ^{3.3}	<input checked="" type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

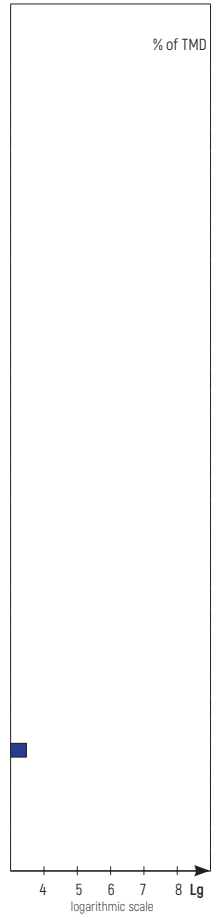

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

DETECTED: Candida spp.

The bacterial microbiome composition is normal.

Example 5. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	10 ^{5.5}	<input type="checkbox"/>
1	Total Bacterial Mass	not detected	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	not detected	
	Commensals, sum	not detected	<input type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>
14	Anaerococcus spp.	not detected	<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	not detected	<input type="checkbox"/>
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
20	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

% of TMD

4 5 6 7 8 Lg
logarithmic scale

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. is below threshold. The bacterial microbiome composition is normal.


WHY IS THERE NO COLOR INDICATION ON THE RESULT FORM?

In example 6, there is no color indication on a report form, as TBM value is $<10^4$. At such low TBM values, relative evaluation is not conducted due to calculation inaccuracies associated with specifics of PCR method. The result of this test is valid, because Human DNA indicator is above the threshold value.

It should be noted that in this case normal microbiota is represented by only one group of bacteria — *Corynebacterium spp.* This sample has a low bacterial load (TBM $<10^5$), so this is a variant of norm.

Example 6. Androflor® Screen assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TBM)
	Human DNA	10 ^{4.5}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{3.8}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{3.1}	
	Commensals, sum	10 ^{3.1}	<input type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
8	Ureaplasma parvum *	not detected	<input type="checkbox"/>
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
11	Candida spp. *	not detected	<input type="checkbox"/>
Sexually transmitted infections			
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

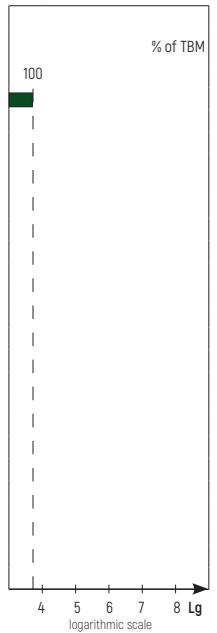

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. DNA is not detected.

The bacterial microbiome composition is normal.

2. The bacterial microbiome composition is abnormal

Disturbance of the balance between normal microbiota and opportunistic microbiota indicates a change in microbiome composition. Depending on the degree of decrease in the normobiota and increase in the proportion of opportunistic microorganisms, the degree of disturbance and the type of proportion of opportunistic microorganisms detected are reported in a conclusion.

ABSOLUTE PREDOMINANCE OF ONE OF THE GROUPS OF NORMAL MICROBIOTA (MICROFLORA)

If normal microbiota is represented by only one group of microorganisms with high enough bacterial load (TBM $>10^5$), an imbalance of the microbiota components is concluded (Example 7).

Presence of more than one group of normal microbiota in samples with high bacterial load (TBM) is considered as norm (Example 1).

Prevalence of one genus is not considered as an imbalance in microbiota in the case of low bacterial load (TBM) (Example 6).

Example 7. Androflor® Screen assay

№	Test title	Result		
		Quantitative	Relative Lg (X/TBM)	
	Human DNA	10 ^{5.8}	<input type="checkbox"/>	
1	Total Bacterial Mass	10 ^{5.1}	<input type="checkbox"/>	
Transit microorganisms				
2	Lactobacillus spp.	not detected	<input type="checkbox"/>	
Commensals				
3	Staphylococcus spp.	not detected		
4	Streptococcus spp.	not detected		
5	Corynebacterium spp.	10 ^{4.9}	-0,2 (54-73%)	
	Commensals, sum	10 ^{4.9}	-0,2 (54-73%)	<input checked="" type="checkbox"/>
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	not detected		<input type="checkbox"/>
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>	
8	Ureaplasma parvum *	not detected	<input type="checkbox"/>	
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>	
	BV-associated opportunistic microorganisms, sum	not detected		<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
10	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{4.0}	-1,1 (7-9%)	<input type="checkbox"/>
Yeast-like fungi				
11	Candida spp. *	below TH ***	<input type="checkbox"/>	
Sexually transmitted infections				
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>	
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>	
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>	
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>	

% of TBM

10 100

4 5 6 7 8 Lg
logarithmic scale

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. is below threshold.

The bacterial microbiome composition is abnormal: the absolute dominance of Corynebacterium spp indicates an imbalance of components of normoflora.

THE BALANCE OF NORMAL AND OPPORTUNISTIC MICROBIOTA (MICROFLORA) IS MODERATELY DISTURBED


WHY DO THE CONCLUSIONS IN THE EXAMPLES BELOW DIFFER?
HOW CAN THE «TOTAL MICROORGANISMS DETECTED» (TMD) INDICATOR BE GREATER THAN 100%?

In examples 8 and 9 bacterial load in the biomaterial samples is low (TBM value $<10^5$), so the degree of imbalance between normal and opportunistic microbiota is not analyzed.

Example 8 is a sample with low bacterial load (TBM $10^{4.3}$). With such low TBM values, it is not possible to correctly «split» TBM into its components due to calculation inaccuracies. It is also important to consider that TBM is determined in a separate tube independently of other parameters in PCR analysis, so minor numerical discrepancies (in the range of method error ± 0.3 lg) are possible, as in this example. The sample reveals «Commensals, sum» (normal microbiota) of $10^{4.5}$ and «Opportunistic anaerobes, sum» of $10^{4.4}$. The percentages in this case are the same. This is an acceptable numerical inaccuracy. The conclusion indicates opportunistic microorganisms presence.

Example 8. Androflor® assay

№	Test title	Result			% of TMD
		Quantitative	Relative Lg (X/TMD)		
	Human DNA	10 ^{5.9}	<input type="checkbox"/>		
1	Total Bacterial Mass	10 ^{4.5}	<input type="checkbox"/>		
Transit microorganisms					
2	Lactobacillus spp.	not detected	<input type="checkbox"/>		
Commensals					
3	Staphylococcus spp.	not detected	<input type="checkbox"/>		
4	Streptococcus spp.	10 ^{4.1}	<input type="checkbox"/>	-0.2 (54-73%)	
5	Corynebacterium spp.	10 ^{4.2}	<input type="checkbox"/>	-0.1 (68-91%)	
	Commensals, sum	10 ^{4.5}	<input type="checkbox"/>	0.2 (85-100%)	
BV-associated opportunistic microorganisms					
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>		
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	10 ^{3.1}	<input type="checkbox"/>	-1.2 (5-7%)	
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>		
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>		
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>		
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>		
12	Atopobium cluster	not detected	<input type="checkbox"/>		
	BV-associated opportunistic microorganisms, sum	10 ^{3.1}	<input type="checkbox"/>	-1.2 (5-7%)	
Opportunistic anaerobes					
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	10 ^{4.0}	<input type="checkbox"/>	-0.3 (43-58%)	
14	Anaerococcus spp.	10 ^{3.5}	<input type="checkbox"/>	-0.8 (13-18%)	
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>		
16	Eubacterium spp.	10 ^{4.1}	<input type="checkbox"/>	-0.2 (54-73%)	
	Opportunistic anaerobes, sum	10 ^{4.4}	<input type="checkbox"/>	0.1 (85-100%)	
Opportunistic microorganisms Haemophilus spp.					
17	Haemophilus spp.	not detected	<input type="checkbox"/>		
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.					
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>		
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.					
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>		
Yeast-like fungi					
20	Candida spp. *	below TH ***	<input type="checkbox"/>		
Sexually transmitted infections					
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>		
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>		
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>		
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>		

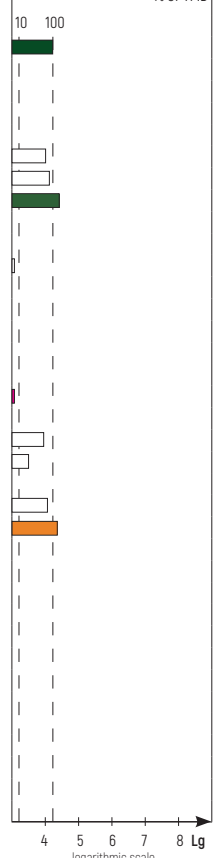

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. is below threshold.

The bacterial microbiome composition is abnormal: opportunistic bacteria are detected.

In example 9, low TBM is detected, the proportion of normal microbiota is reduced and the dominant group in the microbiome composition is anaerobic opportunistic microorganisms.

Example 9. Androflor® assay

№	Test title	Result		% of TMD
		Quantitative	Relative Lg (X/TMD)	
	Human DNA	10 ^{5.4}	<input type="checkbox"/>	
1	Total Bacterial Mass	10 ^{4.2}	<input type="checkbox"/>	
Transit microorganisms				
2	Lactobacillus spp.	not detected	<input type="checkbox"/>	
Commensals				
3	Staphylococcus spp.	not detected		
4	Streptococcus spp.	10 ^{3.4}	-0,8 (13-18%)	
5	Corynebacterium spp.	10 ^{3.5}	-0,7 (17-23%)	
	Commensals, sum	10 ^{3.8}	-0,4 (30-41%)	
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	не выявлено	<input type="checkbox"/>	
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	10 ^{3.3}	-0,9 (11-14%)	
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>	
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>	
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>	
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>	
12	Atopobium cluster	not detected	<input type="checkbox"/>	
	BV-associated opportunistic microorganisms, sum	10 ^{3.3}	-0,9 (11-14%)	
Opportunistic anaerobes				
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>	
14	Anaerococcus spp.	10 ^{3.7}	-0,5 (27-36%)	
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>	
16	Eubacterium spp.	10 ^{3.6}	-0,6 (21-29%)	
	Opportunistic anaerobes, sum	10 ^{4.0}	-0,2 (48-65%)	
Opportunistic microorganisms Haemophilus spp.				
17	Haemophilus spp.	10 ^{3.8}	-0,4 (34-46%)	
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.				
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
19	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{3.4}	-0,8 (13-18%)	
Yeast-like fungi				
20	Candida spp. *	not detected	<input type="checkbox"/>	
Sexually transmitted infections				
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>	
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>	
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>	
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>	

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.


Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: opportunistic bacteria are detected (with opportunistic anaerobes predominance).

In example 10, TBM value exceeds 10^5 , the proportion of normal microflora is reduced, thus the degree of microbiota imbalance is estimated. In this case the balance of normal and opportunistic microbiota is moderately disturbed.

Example 10. Androflor[®] assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TBM)
	Human DNA	$10^{5.7}$	<input type="checkbox"/>
1	Total Bacterial Mass	$10^{5.5}$	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	$10^{4.7}$	-0,5 (27-36%)
4	Streptococcus spp.	$10^{3.9}$	-1,3 (4-6%)
5	Corynebacterium spp.	$10^{3.6}$	-1,6 (2,1-2,9%)
	Commensals, sum	$10^{4.8}$	-0,4 (33-45%)
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	$10^{3.3}$	-1,9 (1,1-1,4%)
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	$10^{3.3}$	-1,9 (1,1-1,4%)
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	$10^{5.6}$	0,4 (85-100%)
14	Anaerococcus spp.	$10^{3.7}$	-1,5 (3-4%)
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	$10^{3.6}$	-1,6 (2,1-2,9%)
	Opportunistic anaerobes, sum	$10^{5.6}$	0,4 (85-100%)
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	$10^{4.3}$	-0,9 (11-14%)
Yeast-like fungi			
20	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

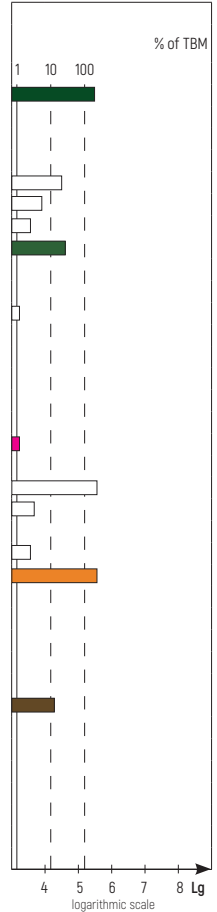

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. is below threshold.

The bacterial microbiome composition is abnormal: the balance of normal and opportunistic microflora is moderately disturbed.

THE BALANCE OF NORMAL AND OPPORTUNISTIC MICROBIOTA (MICROFLORA) IS SEVERELY DISTURBED

If normal microbiota is present in a sample in low quantity and the biotope is dominated by opportunistic microorganisms, it is reported that the balance of normal and opportunistic microbiota is significantly disturbed (Examples 11, 12 and 13).

In example 12, a pathogenic microorganism (*Mycoplasma genitalium*) was also detected in a sample, which is reported in the conclusion along with the information about microbiota imbalance.

Example 11. Androflor® Screen assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	10 ^{4,8}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{5,4}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{3,4}	-2,0 [0,8-1,1%]
	Commensals, sum	10 ^{3,4}	-2,0 [0,8-1,1%] ■
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	10 ^{5,2}	-0,2 [54-73%] ■
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
8	Ureaplasma parvum *	not detected	<input type="checkbox"/>
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	10 ^{5,2}	-0,2 [54-73%] ■
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{4,8}	-0,5 [27-36%] ■
Yeast-like fungi			
11	Candida spp. *	not detected	<input type="checkbox"/>
Sexually transmitted infections			
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

logarithmic scale

4 5 6 7 8 Lg

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:


STIs DNA is not detected.

Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: the balance of normal and opportunistic microflora is severely disturbed (with BV-associated opportunistic microorganisms predominance).

Example 12. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	10 ^{4.6}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{6.4}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	10 ^{3.2}	-3,2 (<0,1%) <input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	10 ^{3.9}	-2,5 [0,3-0,4%]
4	Streptococcus spp.	10 ^{3.5}	-2,9 [0,1-0,1%]
5	Corynebacterium spp.	10 ^{4.5}	-1,9 [1,1-1,4%]
	Commensals, sum	10 ^{4.6}	-1,8 [1,4-2,0%] <input checked="" type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	не выявлено	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	10 ^{5.2}	-1,2 [5-7%] <input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	10 ^{3.5}	-2,9 [0,1-0,1%] <input type="checkbox"/>
9	Ureaplasma urealyticum *	не выявлено	<input type="checkbox"/>
10	Ureaplasma parvum *	не выявлено	<input type="checkbox"/>
11	Mycoplasma hominis *	не выявлено	<input type="checkbox"/>
12	Atopobium cluster	не выявлено	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	10 ^{5.2}	-1,2 [5-7%] <input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	10 ^{6.1}	-0,3 [43-58%] <input checked="" type="checkbox"/>
14	Anaerococcus spp.	10 ^{4.7}	-1,7 [1,7-2,3%] <input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	10 ^{4.5}	-1,9 [1,1-1,4%] <input type="checkbox"/>
16	Eubacterium spp.	10 ^{5.1}	-1,3 [4-6%] <input type="checkbox"/>
	Opportunistic anaerobes, sum	10 ^{6.2}	-0,2 [50-67%] <input checked="" type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	не выявлено	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	не выявлено	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{5.9}	-0,5 [27-36%] <input checked="" type="checkbox"/>
Yeast-like fungi			
20	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	DETECTED	<input checked="" type="checkbox"/>
22	Trichomonas vaginalis **	не выявлено	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	не выявлено	<input type="checkbox"/>
24	Chlamydia trachomatis **	не выявлено	<input type="checkbox"/>

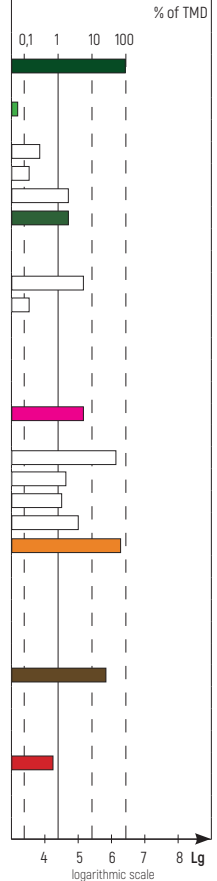

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:


DETECTED: Mycoplasma genitalium.

Candida spp. is below threshold.

The bacterial microbiome composition is abnormal: STIs DNA is detected, the balance of normal and opportunistic microflora is severely disturbed.

Example 13. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	10 ^{5.8}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{5.7}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	10 ^{4.3}	-1.2 (5-7%)
4	Streptococcus spp.	not detected	<input type="checkbox"/>
5	Corynebacterium spp.	10 ^{5.9}	-1.6 (2.1-2.9%)
	Commensals, sum	10 ^{4.4}	-1.1 (7-10%) ■
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>
14	Anaerococcus spp.	not detected	<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	not detected	<input type="checkbox"/>
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{5.7}	0.2 (85-100%) ■
Yeast-like fungi			
20	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

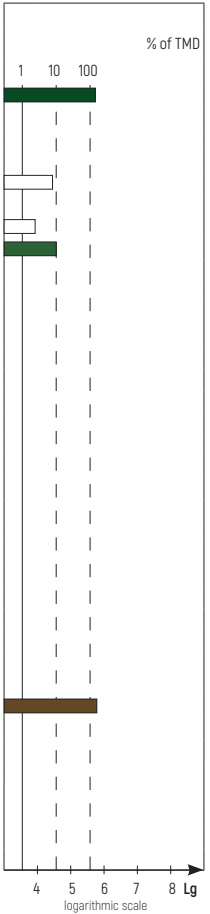

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. is below threshold.

The bacterial microbiome composition is abnormal: the balance of normal and opportunistic microflora is severely disturbed (with Enterobacteriaceae spp. / Enterococcus spp. predominance).

SIGNIFICANT DECREASE/ABSENCE OF NORMAL MICROFLORA IS NOT PROPORTIONAL TO THE ABSENCE/SLIGHT INCREASE OF OPPORTUNISTIC MICROFLORA

In example 14, the decrease in normal microbiota is not proportional to the increase in opportunistic microorganisms (OMs). The analysis was performed with Androflor® Screen, which is intended for screening and does not include the full range of OMs. At the physician's decision, an additional examination can be performed using the Androflor® assay with an extended list of OMs.

Example 14. Androflor® Screen assay

№	Test title	Result	
		Quantitative	Relative Lg [X/TBM]
	Human DNA	10 ^{5.2}	<input type="checkbox"/>
1	Total Bacterial Mass	10 ^{6.2}	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	10 ^{3.5}	-2,7 (0,2-0,2%)
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{4.2}	-2,0 (0,8-1,1%)
	Commensals, sum	10 ^{4.3}	-1,9 (1,0-1,4%)
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
8	Ureaplasma parvum *	not detected	<input type="checkbox"/>
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
10	Enterobacteriaceae spp. / Enterococcus spp.	10 ^{5.5}	-0,7 (1,7-23%)
Yeast-like fungi			
11	Candida spp. *	not detected	<input type="checkbox"/>
Sexually transmitted infections			
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

% of TBM

logarithmic scale

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. DNA is not detected.

The bacterial microbiome composition is abnormal: decrease/absence of normal microflora is not proportional to the absence/slight increase of opportunistic microflora.

In example 15, a male urethral scrape was analyzed using the Androflor® assay. The TBM value of $10^{4.7}$ was obtained, and no microorganisms were detected that are included in the analytes list of the assay. This indicates that some microorganism was present in this sample that is not specifically detected by the Androflor® test system. Upon further investigation by sequencing, *Treponema pallidum* was identified.

Example 15. Androflor® assay

№	Test title	Result		% of TMD
		Quantitative	Relative Lg [X/TMD]	
	Human DNA	$10^{4.2}$	<input type="checkbox"/>	
1	Total Bacterial Mass	$10^{4.7}$	<input type="checkbox"/>	
Transit microorganisms				
2	Lactobacillus spp.	not detected	<input type="checkbox"/>	
Commensals				
3	Staphylococcus spp.	not detected		
4	Streptococcus spp.	not detected		
5	Corynebacterium spp.	not detected		
	Commensals, sum	not detected	<input type="checkbox"/>	
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>	
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>	
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>	
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>	
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>	
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>	
12	Atopobium cluster	not detected	<input type="checkbox"/>	
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>	
Opportunistic anaerobes				
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>	
14	Anaerococcus spp.	not detected	<input type="checkbox"/>	
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>	
16	Eubacterium spp.	not detected	<input type="checkbox"/>	
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Haemophilus spp.				
17	Haemophilus spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.				
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>	
Yeast-like fungi				
20	Candida spp. *	below TH ***	<input type="checkbox"/>	
Sexually transmitted infections				
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>	
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>	
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>	
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>	

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.
 Candida spp. is below threshold.
 The bacterial microbiome composition is abnormal: decrease/absence of normal microflora is not proportional to the absence/slight increase of opportunistic microflora.

STIS' DNA IS DETECTED (OBLIGATE PATHOGENS ARE PRESENT)

In example 16, Human DNA is present while TBM is absent. This result is considered as valid. At the same time, *Mycoplasma genitalium* and *Candida spp.* are detected in significant amounts, i.e. the microbiome composition is abnormal.

Example 16. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg [X/TMD]
	Human DNA	10 ^{5.8}	<input type="checkbox"/>
1	Total Bacterial Mass	not detected	<input type="checkbox"/>
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	not detected	
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	not detected	
	Commensals, sum	not detected	<input type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>
14	Anaerococcus spp.	not detected	<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	not detected	<input type="checkbox"/>
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
20	Candida spp. *	10 ^{5.2}	<input checked="" type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	DETECTED	<input checked="" type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

% of TMD

logarithmic scale

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

DETECTED: Mycoplasma genitalium.

DETECTED: Candida spp.


The bacterial microbiome composition is abnormal: STIs DNA is detected.

3. Cases when no conclusion is issued

INSUFFICIENT AMOUNT OF BIOMATERIAL: TBM AND HUMAN DNA ARE BOTH NOT DETECTED OR BELOW THRESHOLD

Example 17. Androflor® assay

№	Test title	Result	
		Quantitative	Relative Lg (X/TMD)
	Human DNA	not detected	■
1	Total Bacterial Mass	10 ^{3.4}	■
Transit microorganisms			
2	Lactobacillus spp.	not detected	<input type="checkbox"/>
Commensals			
3	Staphylococcus spp.	10 ^{3.2}	-2.2 (54-73%)
4	Streptococcus spp.	not detected	
5	Corynebacterium spp.	10 ^{3.2}	-0.2 (54-73%)
	Commensals, sum	10 ^{3.5}	0.1 (85-100%) <input type="checkbox"/>
BV-associated opportunistic microorganisms			
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>
10	Ureaplasma parvum *	10 ^{3.4}	■
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>
12	Atopobium cluster	not detected	<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>
Opportunistic anaerobes			
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>
14	Anaerococcus spp.	not detected	<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>
16	Eubacterium spp.	not detected	<input type="checkbox"/>
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.			
17	Haemophilus spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.			
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.			
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>
Yeast-like fungi			
20	Candida spp. *	below TH ***	<input type="checkbox"/>
Sexually transmitted infections			
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected	<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>

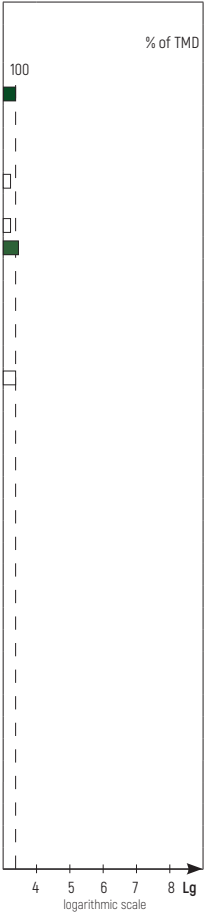

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

Amount of bacterial and/or human DNA in the sample is not enough for the test result.

EXCEEDING THE THRESHOLD VALUES OF TRANSIENT MICROBIOTA (MICROFLORA)

In cases when transient microbiota accounts for more than 10% of the bacterial load of a biotope, a conclusion on microbiome composition is not issued. At a physician's decision, it is possible to repeat biomaterial sampling under the condition of protected sexual contacts or sexual abstinence for 3 days.

Example 18. Androflor® Screen assay

№	Test title	Result		% of TBM
		Quantitative	Relative Lg (X/TBM)	
	Human DNA	10 ^{4.8}	<input type="checkbox"/>	
1	Total Bacterial Mass	10 ^{4.3}	<input type="checkbox"/>	
Transit microorganisms				
2	Lactobacillus spp.	10 ^{3.8}	-0.5 (27-36%)	<input checked="" type="checkbox"/>
Commensals				
3	Staphylococcus spp.	10 ^{3.1}	-1.2 (5-7%)	<input type="checkbox"/>
4	Streptococcus spp.	not detected		<input type="checkbox"/>
5	Corynebacterium spp.	10 ^{3.5}	-0.8 (13-18%)	<input type="checkbox"/>
	Commensals, sum	10 ^{3.6}	-0.7 (19-25%)	<input checked="" type="checkbox"/>
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	not detected		<input type="checkbox"/>
7	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>	
8	Ureaplasma parvum *	not detected	<input type="checkbox"/>	
9	Mycoplasma hominis *	not detected	<input type="checkbox"/>	
	BV-associated opportunistic microorganisms, sum	not detected		<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
10	Enterobacteriaceae spp. / Enterococcus spp.	not detected		<input type="checkbox"/>
Yeast-like fungi				
11	Candida spp. *	not detected	<input type="checkbox"/>	
Sexually transmitted infections				
12	Mycoplasma genitalium **	not detected	<input type="checkbox"/>	
13	Trichomonas vaginalis **	not detected	<input type="checkbox"/>	
14	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>	
15	Chlamydia trachomatis **	not detected	<input type="checkbox"/>	

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. DNA is not detected.

Exceeding the threshold values of transient microflora does not allow to make a correct conclusion about the real composition of the bacterial microbiome belong to patient. Microflora e.g. BV-associated bacteria, can be the cause of acute inflammation of the lower parts of the urogenital tract. The result of the study directly depends on compliance with the rules of preparation for the collection of biomaterial.

In example 19, *Gardnerella vaginalis* was also detected in significant numbers, in addition to *Lactobacillus spp.*, despite meeting all pre-analytical requirements for repeated biomaterial sampling. In this case, *Lactobacillus spp.* and *Gardnerella vaginalis* are predominant components of a male patient's microbiota and may be a cause of acute inflammation in the lower urogenital tract [1].

Example 19. Androflor® assay

№	Test title	Result		% of TMD
		Quantitative	Relative Lg (X/TMD)	
	Human DNA	10 ^{5.7}	<input type="checkbox"/>	
1	Total Bacterial Mass	10 ^{5.5}	<input type="checkbox"/>	
Transit microorganisms				
2	Lactobacillus spp.	10 ^{5.6}	0,1 (85-100%)	<input checked="" type="checkbox"/>
Commensals				
3	Staphylococcus spp.	10 ^{3.9}	-1,6 (2,1-2,9%)	<input type="checkbox"/>
4	Streptococcus spp.	10 ^{3.6}	-1,9 (1,1-1,4%)	<input type="checkbox"/>
5	Corynebacterium spp.	10 ^{3.8}	-1,7 (1,7-2,3%)	<input type="checkbox"/>
	Commensals, sum	10 ^{4.3}	-1,2 (5-7%)	<input checked="" type="checkbox"/>
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	10 ^{5.4}	-0,1 (68-91%)	<input checked="" type="checkbox"/>
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected		<input type="checkbox"/>
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected		<input type="checkbox"/>
9	Ureaplasma urealyticum *	not detected		<input type="checkbox"/>
10	Ureaplasma parvum *	not detected		<input type="checkbox"/>
11	Mycoplasma hominis *	not detected		<input type="checkbox"/>
12	Atopobium cluster	not detected		<input type="checkbox"/>
	BV-associated opportunistic microorganisms, sum	10 ^{5.4}	-0,1 (68-91%)	<input checked="" type="checkbox"/>
Opportunistic anaerobes				
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected		<input type="checkbox"/>
14	Anaerococcus spp.	not detected		<input type="checkbox"/>
15	Peptostreptococcus spp. / Parvimonas spp.	not detected		<input type="checkbox"/>
16	Eubacterium spp.	10 ^{4.8}	-0,7 (17-23%)	<input checked="" type="checkbox"/>
	Opportunistic anaerobes, sum	10 ^{4.8}	-0,7 (17-23%)	<input checked="" type="checkbox"/>
Opportunistic microorganisms Haemophilus spp.				
17	Haemophilus spp.	not detected		<input type="checkbox"/>
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.				
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected		<input type="checkbox"/>
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected		<input type="checkbox"/>
Yeast-like fungi				
20	Candida spp. *	not detected		<input type="checkbox"/>
Sexually transmitted infections				
21	Mycoplasma genitalium **	not detected		<input type="checkbox"/>
22	Trichomonas vaginalis **	not detected		<input type="checkbox"/>
23	Neisseria gonorrhoeae **	not detected		<input type="checkbox"/>
24	Chlamydia trachomatis **	not detected		<input type="checkbox"/>

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:

STIs DNA is not detected.

Candida spp. DNA is not detected.

Exceeding the threshold values of transient microflora does not allow to make a correct conclusion about the real composition of the bacterial microbiome belong to patient. Microflora e.g. BV-associated bacteria, can be the cause of acute inflammation of the lower parts of the urogenital tract. The result of the study directly depends on compliance with the rules of preparation for the collection of biomaterial.

[1] Pochernikov DG, Postovoytenko NT, Getman VV, Galkina IS. Diagnostic significance of Lactobacillus spp. identification in ejaculate. Bulletin of RSMU, 2020, 3. DOI: 10.204075/vrgmu.2020.039

WILL OBLIGATE PATHOGENS BE DETECTED, IF HUMAN DNA AND TBM ARE NOT DETECTED?

Even if TBM and Human DNA are both below the threshold values, or if transient microflora is present at more than 10% of TBM, information on the detected obligate pathogens will be reported in the automated conclusion. The microbiome composition will not be analyzed (Example 20).

Example 20. Androflor® assay

№	Test title	Result		% of TBM
		Quantitative	Relative Lg (X/TBM)	
	Human DNA	not detected	■	
1	Total Bacterial Mass	not detected	■	
Transit microorganisms				
2	Lactobacillus spp.	not detected	<input type="checkbox"/>	
Commensals				
3	Staphylococcus spp.	not detected		
4	Streptococcus spp.	not detected		
5	Corynebacterium spp.	10 ^{3.3}		
	Commensals, sum	10 ^{3.3}	<input type="checkbox"/>	
BV-associated opportunistic microorganisms				
6	Gardnerella vaginalis	not detected	<input type="checkbox"/>	
7	Megasphaera spp. / Veillonella spp. / Dialister spp.	not detected	<input type="checkbox"/>	
8	Sneathia spp. / Leptotrichia spp. / Fusobacterium spp.	not detected	<input type="checkbox"/>	
9	Ureaplasma urealyticum *	not detected	<input type="checkbox"/>	
10	Ureaplasma parvum *	not detected	<input type="checkbox"/>	
11	Mycoplasma hominis *	not detected	<input type="checkbox"/>	
12	Atopobium cluster	not detected	<input type="checkbox"/>	
	BV-associated opportunistic microorganisms, sum	not detected	<input type="checkbox"/>	
Opportunistic anaerobes				
13	Bacteroides spp. / Porphyromonas spp. / Prevotella spp.	not detected	<input type="checkbox"/>	
14	Anaerococcus spp.	not detected	<input type="checkbox"/>	
15	Peptostreptococcus spp. / Parvimonas spp.	not detected	<input type="checkbox"/>	
16	Eubacterium spp.	not detected	<input type="checkbox"/>	
	Opportunistic anaerobes, sum	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Haemophilus spp.				
17	Haemophilus spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.				
18	Pseudomonas aeruginosa / Ralstonia spp. / Burkholderia spp.	not detected	<input type="checkbox"/>	
Opportunistic microorganisms Enterobacteriaceae spp. / Enterococcus spp.				
19	Enterobacteriaceae spp. / Enterococcus spp.	not detected	<input type="checkbox"/>	
Yeast-like fungi				
20	Candida spp. *	below TH ***	<input type="checkbox"/>	
Sexually transmitted infections				
21	Mycoplasma genitalium **	not detected	<input type="checkbox"/>	
22	Trichomonas vaginalis **	DETECTED	■	
23	Neisseria gonorrhoeae **	not detected	<input type="checkbox"/>	
24	Chlamydia trachomatis **	not detected	<input type="checkbox"/>	

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

4 5 6 7 8 Lg
logarithmic scale

Conclusion:

DETECTED: Trichomonas vaginalis.



e206-1 2023.12.28



DNA-TECHNOLOGY