513-3 2022-08-25

For professional use only

Femoflor® 16 REAL-TIME PCR Detection Kit

INSTRUCTION FOR USE

OBELIS S.A

Registered Address:

Bd. Général Wahis, 53

1030 Brussels, Belgium

Tel: +32.2.732.59.54

Fax: +32.2.732.60.03

E-mail: mail@obelis.net

http://www.obelis.net

"DNA-Technology Research & Production", LLC,

142281, Russia,

Moscow Region, Protvino,

Zheleznodorozhnaya Street, 20

Phone/fax: +7(495) 640.17.71

E-mail: info@dna-technology.com

https://www.dna-technology.com

Customer service department

E-mail: hotline@dna-technology.ru

REF R1-P801-S3/6EU

VER 513-3.2022.08.25

TABLE OF CONTENTS

1. INTENDED USE	**3**
2. METHOD	**3**
3. CONTENT	**5**
4. REAGENTS AND EQUIPMENT REQUIRED BUT NOT PROVIDED	**5**
5. TRANSPORT AND STORAGE CONDITIONS	**6**
6. WARNINGS AND PRECAUTIONS	**7**
7. SAMPLES	**8**
8. PROCEDURE	**10**
9. CONTROLS	**12**
10. DATA ANALYSIS	**12**
11. SPECIFICATIONS	**14**
12. TROUBLESHOOTING	**15**
13. QUALITY CONTROL	**16**
14. KEY TO SYMBOLS	**17**

1. INTENDED USE

The **Femoflor® 16 REAL-TIME PCR Detection Kit** offers an *in vitro* nucleic acid based test. The test utilizes the Polymerase Chain Reaction (PCR) nucleic acid amplification technique aimed to detect opportunistic flora and normal flora in urogenital specimens.

The **Femoflor® 16 REAL-TIME PCR Detection Kit** allows, using one biological sample, to perform a quantitative assessment of the total bacterial mass, urogenital normoflora - lactobacilli, complex of aerobic and anaerobic microorganisms, typical for the women's urogenital tract, mycoplasmas, fungi of the Candida genus, involved in the development of dysbiotic processes in urogenital microbiome composition.

The microbiome state has a serious impact on the reproductive function and, as a result, on the quality of woman's life. Diseases caused by opportunistic microflora may occur both with clinical manifestations and asymptomatically. The asymptomatic disease course often leads to late reference to doctor and development of serious complications. Diseases caused by opportunistic microorganisms increase the risk of infection with sexually transmitted infections and HIV infections. In time undiagnosed infections, associated with a opportunistic microflora, can cause abnormalities in the women reproductive function, spontaneous abortions, premature births, intrauterine infection and low fetal birth weight, postnatal complications, and complications after surgery intervention on the pelvic organs. The urgency of diagnostics of the opportunistic microflora associated infections of urogenital tract is in question. The diagnostic methods used in routine laboratory practice do not always allow the doctor to adequately assess the patient's condition and prescribe the necessary treatment. At the same time, the possibilities of the modern PCR laboratory allow to conduct the multifactorial quantitative studies, detecting the DNA of various microorganisms in the samples.

The application of the kit does not depend on population and demographic aspects. There are no contradictions for use of the **Femoflor® 16 REAL-TIME PCR Detection Kit.**

The **Femoflor® 16 REAL-TIME PCR Detection Kit** can be used in clinical and diagnostic laboratories of medical institutions and research practice.

Potential users: personnel qualified in molecular diagnostics methods and working in the clinical and diagnostic laboratory.

It is necessary to apply the kit only as directed in this instruction for use.

2. METHOD

The implemented PCR method is based on amplification of a target DNA sequence. To increase the sensitivity and specificity of the amplification reaction, the use of a hot-start is provided. Hot-start is provided by reaction mixture preparation consisting of two layers separated by a layer of paraffin or the use of Taq-polymerase blocked by antibodies. The polymerase chain reaction starts only when paraffin is melted or thermal dissociation of a complex of Taq polymerase and antibodies is happened. It excludes non-specific annealing of primers to targets DNA in the initial heating of the tube.

The **Femoflor® 16® REAL-TIME PCR Detection Kit** is based on fluorescent modification of the PCR method. The PCR-mix contains two target-specific probes bearing reporter fluorescent dyes (Fam and Hex) and quencher molecules. Once hybridized to a target sequence, the probes become activated. As a result of activation fluorescence increases proportionally to target sequence amplification. The intensity of fluorescence is measured at every cycle of reaction with a Real-time PCR thermal cycler data collection unit and analyzed with the software provided.

The **Femoflor® 16 REAL-TIME PCR Detection Kit** includes following components: PCR-mixes for total bacterial mass amplification, PCR-mixes for Lactobacillus spp. amplification, PCR-mixes for opportunistic flora DNA amplification.

One tube (strip-2, tube №8) contains a PCR-mix for the amplification of human genomic DNA (sample intake control (SIC)). The SIC allows to exclude preanalytical error. If the amount of collected material is insufficient for the analysis, it is necessary to repeat sampling procedure.

One tube (strip-1, tube №2) contains an internal control (IC), which is intended to assess the quality of the polymerase chain reaction.

The fluorescent dyes are assigned to individual types of sequences. The Fam dye label is used to detect specific sequences. The Hex dye label is used to detect SIC and IC. Use of two distinguishable dyes allows detection of both PCR products simultaneously.

Defined tubes contain additional probe with Rox dye label – "Marker". It tags the strip orientation. Upon completion of run, software defines actual position of the strip (by means of "marker" position) relative to the position preset by the operator. If it mismatches, the software suggests rearrangement of the tubes by default. In accordance with the operator, order can be rearranged and saved in new file.

Upon completion of the run, software performs relative quantitative analysis of total bacterial DNA, genus-specific DNA of Lactobacillus spp. and genus/species-specific DNA of each the opportunistic pathogens (or flora). To exclude false negatives, human DNA (SIC) quantity is considered. Table 1 shows the detection channels of amplification products.

Table 1. Detection channels of amplification products for **Femoflor® 16 REAL-TIME PCR Detection Kit**

№ of tube in a strip	Dye label/detection channel			**Color labeling of the buffer**	**Color labeling of the paraffin**
	Fam	**Hex**	**Rox**		
Strip-1					
1	Total bacterial mass (TBM)	-	-	Blue	White
2	*Lactobacillus* spp.	IC	-	Colorless	
3	*Enterobacteriaceae*	-	-		
4	*Streptococcus* spp.	-	-		
5	*Staphylococcus* spp.	-	Marker		
6	*Gardnerella vaginalis*/*Prevotella bivia*/*Porphyromonas* spp.	-	-		
7	*Eubacterium* spp.	-	-		
8	*Sneathia* spp./*Leptotrihia* spp./ *Fusobacterium* spp.	-	-		
Strip-2					
1	*Megasphaera* spp./*Veilonella* spp./ *Dialister* spp.	-	-	Blue	Blue
2	*Lachnobacterium* spp./ *Clostridium* spp.	-	-	Colorless	
3	*Mobiluncus* spp./ *Corynebacterium* spp.	-	-		
4	*Peptostreptococcus spp.*	-	-		
5	*Atopobium vaginae*	-	-		
6	*Mycoplasma hominis*	*Mycoplasma genitalium*	-		
7	*Ureaplasma (urealyticum + parvum)*	-	-		
8	*Candida* spp.	SIC	Marker		

The automatic analysis is available on "DNA-Technology" made instruments: DTlite or DTprime REAL-TIME Thermal Cyclers (see the catalogue at https://www.dna-technology.com to see available supply options). The current version of the software is available for download at https://www.dna-technology.com/software.

3. CONTENT

The **Femoflor® 16 REAL-TIME PCR Detection Kit** content is represented in Table 2.

Table 2. The **Femoflor® 16 REAL-TIME PCR Detection Kit** content, package S (standard)

Reagent	Description	Total volume	Amount
Paraffin sealed PCR-mix	Colorless or blue transparent liquid under waxy white or blue fraction	3840 µL (20 µL in each tube)	24 8-tube strips
Taq-polymerase solution	Colorless transparent liquid	2000 µL (500 µL in each tube)	4 tubes
Mineral oil	Colorless transparent viscous oily liquid	4.0 mL (1.0 mL in each tube)	4 tubes
Positive control	Colorless transparent liquid	160 µL	1 tube
Strip's caps	24 8-caps		

All components are ready to use and do not require additional preparation for operation.

The **Femoflor® 16 REAL-TIME PCR Detection Kit** is intended for single use and designed for 12 tests (no more than 10 defined samples, one positive control and one negative control).

4. REAGENTS AND EQUIPMENT REQUIRED BUT NOT PROVIDED

4.1. Specimen collection

- Specimen collection swabs: use only dacron, rayon, or calcium alginate tipped collection swabs with plastic or non-aluminum wire shafts;
- Sterile tubes containing transport media: "DNA-Technology" made **PREP-RAPID** (REF P-001/1EU not applicable to male urethral smears) or **STOR-M** (REF P-910-1/1EU) or **STOR-F** (REF P-901-1/1EU, P-901-N/1EU, P-901-R/1EU) or equivalent or physiological saline solution or sterile PBS for the transportation of the sample.

4.2. DNA extraction and PCR

Preamplification-specimen and control preparation area:

- Biological safety cabinet class II;
- Refrigerator;
- Vortex mixer;
- High speed centrifuge (RCF(g) no less than 16000);
- Solid-state thermostat (temperature range 50-65 °C);
- Tube rack for 1.5 mL tubes;
- 1.5 mL tubes;
- Single channel pipettes (dispensers covering 20-1000 µL volume range);
- RNase and DNase free filtered pipette tips (volume 200 µL, 1000 µL);
- Electric laboratory aspirator with trap flask for the removal of supernatant;
- RNase and DNase free non-filtered pipette tips for aspirator with trap flask;
- Nucleic acid extraction kit ("DNA-Technology" made **PREP-NA PLUS** (REF P-002/2EU) or **PREP-GS PLUS** (REF P-003/2EU) and **PREP-MB RAPID** (REF P-116-A/8EU) extraction kits are recommended);

- Physiological saline solution 0.9% NaCl (Sterile);
- Container for used pipette tips, tubes and other consumables;
- Powder-free surgical gloves;
- Disinfectant solution.

Preamplification-reagent preparation area:

- UV PCR cabinet;
- Refrigerator;
- Vortex mixer;
- Vortex rotor for strips;
- PCR tube rack for 0.2 mL tubes in strips;
- Single channel pipettes (dispensers covering 2.0-1000 µL volume range);
- RNase and DNase free filtered pipette tips (volume 20 µL, 200 µL, 1000 µL);
- Container for used pipette tips, tubes and other consumables;
- Powder-free surgical gloves;
- Disinfectant solution.

Post-Amplification – Amplification detection area:

- Real-time PCR thermal cycler.

Software:

The most recent version of the DT thermal cyclers software can be downloaded from https://www.dna-technology.com/software.

The OS supported: all versions of Windows starting from 7.

5. TRANSPORT AND STORAGE CONDITIONS

Expiry date – 12 months from the date of production.

All components of the **Femoflor® 16 REAL-TIME PCR Detection Kit** must be stored at temperatures from 2 °C to 8 °C during the storage period. PCR-mix must be stored at temperatures from 2 °C to 8 °C and out of light during the storage period. The excessive temperature and light can be detrimental to product performance.

The kit transportation can be held by all types of roofed transport at temperatures from 2 °C to 8 °C over the transportation. It is allowed to transport the kit at temperatures from 2 °C to 8 °C for no more than 5 days.

Shelf-life of the kit following the first opening of the primary container:
- components of the kit should be stored at temperatures from 2 °C to 8 °C during the storage period;
- PCR-mix for amplification should be stored at temperatures from 2 °C to 8 °C and out of light during the storage period.

The kit stored in under undue regime should not be used.

An expired the **Femoflor® 16 REAL-TIME PCR Detection Kit** should not be used.

We strongly recommend to follow the given instructions in order to obtain accurate and reliable results.

The conformity of the **Femoflor® 16 REAL-TIME PCR Detection Kit** to the prescribed technical requirements is subject to compliance of storage, transportation and handling conditions recommended by manufacturer.

6. WARNINGS AND PRECAUTIONS

Only personnel trained in the methods of molecular diagnostics and the rules of work in the clinical and diagnostic laboratory are allowed to work with the kit.

Handle and dispose all biological samples, reagents and materials used to carry out the assay as if they were able to transmit infective agents. The samples must be exclusively employed for certain type of analysis. Samples must be handled under a laminar flow hood. Tubes containing different samples must never be opened at the same time. Pipettes used to handle samples must be exclusively employed for this specific purpose. The pipettes must be of the positive dispensation type or be used with aerosol filter tips. The tips employed must be sterile, free from the DNases and RNases, free from DNA and RNA. The reagents must be handled under a laminar flow hood. The reagents required for amplification must be prepared in such a way that they can be used in a single session. Pipettes used to handle reagents must be exclusively employed for this specific purpose. The pipettes must be of the positive dispensation type or be used with aerosol filter tips. The tips employed must be sterile, free from the DNases and RNases, free from DNA and RNA. The reagents must be handled under a laminar flow hood. The reagents required for amplification must be prepared in such a way that they can be used in a single session. Pipettes used to handle reagents must be exclusively employed for this specific purpose. The pipettes must be of the positive dispensation type or be used with aerosol filter tips. The tips employed must be sterile, free from the DNases and RNases, free from DNA and RNA**.** Avoid direct contact with the biological samples reagents and materials used to carry out the assay. Wear powder-free surgical gloves. Wear protective clothing (work clothes and personal protective equipment) working with microorganisms classified as particularly pathogenic. The protective clothing and personal protective equipment must comply with the work to be performed and health and safety requirements. Avoid producing spills or aerosol. Any material being exposed to biological samples must be treated for at least 30 minutes with disinfecting solution or autoclaved for 1 hour at 121 °C before disposal.

Molecular biology procedures, such as nucleic acids extraction, PCR-amplification and detection require qualified staff to avoid the risk of erroneous results, especially due to the degradation of nucleic acids contained in the samples or sample contamination by amplification products.

All oligonucleotide components are produced by artificial synthesis technology according to internal quality control protocol and do not contain blood or products of blood processing.

Positive control is produced by artificial DNA synthesis technology. Positive control does not include parts of infectious agents.

All the liquid solutions are designed for single use and can not be used more than once in amplification reactions. Plastic tubes do not contain phthalates. Do not breathe gas/fumes/vapor/spray produced by the components of the kit. Do not eat/drink components of the kit. Avoid contact with eyes. Only use the reagents provided in the kit and those recommended by manufacturer. Do not mix reagents from different batches. Do not use reagents from third party manufacturers' kits. All laboratory equipment, including pipettes, test tube racks, laboratory glassware, lab coats, bouffant caps, etc., as well as reagents should be strictly stationary. It is not allowed to move them from one room to another. Equip separate areas for the extraction/preparation of amplification reactions and for the amplification/detection of amplification products. Never introduce an amplification product in the area designed for extraction/preparation of amplification reactions. Wear lab coats, gloves and tools, which are exclusively employed for the extraction/preparation of the amplification reaction and for the amplification/detection of the amplification products. Never transfer lab coats, gloves and tools from the area designed for amplification/detection of the amplification products to the area designed for extraction/preparation of amplification reactions. Amplification products must be handled in such a way as to reduce dispersion into the environment as much as possible, in order to avoid the possibility of contamination. Pipettes used to handle amplification products must be exclusively employed for this specific purpose. Remove PCR waste only in a closed form. Remove waste materials (tubes, tips) only in a special closed container containing a disinfectant solution. Work surfaces, as well as rooms where NA extraction and PCR are performed, must be irradiated with bactericidal irradiators for 30 minutes before and after the work.

Do not open the tubes after amplification. Waste materials are disposed of in accordance with local and national standards. All surfaces in the laboratory (work tables, test tube racks, equipment, etc.) must be treated daily with disinfecting solution.

Emergency actions

Inhalation: Inhalation of the PCR-mix contained within this kit is unlikely, however care should be taken.

Eye Contact: If any component of this kit enters the eyes, wash eyes gently under potable running water for 15 minutes or longer, making sure that the eyelids are held open. If pain or irritation occurs, obtain medical attention.

Skin Contact: If any component of this kit contacts the skin and causes discomfort, remove any contaminated clothing. Wash affected area with plenty of soap and water. If pain or irritation occurs, obtain medical attention.

Ingestion: If any component of this kit is ingested, wash mouth out with water. If irritation or discomfort occurs, obtain medical attention.

Do not use the kit:

- When the transportation and storage conditions are breached;
- When the reagents' appearance does not respond to the kit passport;
- When the kit components packaging is breached;
- After the expiry date provided.

Significant health effects are **NOT** anticipated from routine use of this kit when adhering to the instructions listed in the current manual.

7. SAMPLES

The **Femoflor® 16 REAL-TIME PCR Detection Kit** is designed to detect DNA extracted from epithelial scrapes from cervical canal, posterolateral vaginal vault and urethra, depending on professional prescription.

General requirements

To interpret results successfully and robustly, a high quality of sample and appropriate conditions of storage, transport, and handling are required.

PCR analysis refers to direct methods of laboratory research; therefore the collection of biological material must be carried out from the site of infection localization.

A biological sample is analyzed for the presence and quantity of the normo- and opportunistic microorganisms DNA. At the same time, the sampling quality is assessed by quantitative evaluation of human genomic DNA.

Sample collection and preparation

Professional prescription is required to localize the place of sampling (urethra, cervix or vaginal wall). The decision must be based on a patient's complaints and clinical signs, and made by the physician in charge.

Women must not perform hygiene procedures or syringing prior the sampling procedure.

To interpret results successfully and robustly, sample must contain the largest possible number of epithelial cells with minimum amounts of mucus and blood. Inappropriate sampling may result in doubtful results and sample collection may need to be repeated.

Sampling, sample processing procedures and storage are carried out in accordance with the instructions to the DNA extraction kit from biological material.

Urogenital scrapes sampling

The urogenital sampling is held by sterile swab (or brush). The sample is then transferred to the 1.5 mL plastic tubes containing 300 µL of physiological saline solution or in the tubes containing transport media, for example “DNA-Technology” made **PREP-RAPID** or **STOR-M** or **STOR-F**.

The features of the vaginal sampling:

The sample must be taken prior to physical inspection. Speculum can be treated by warm sterile saline solution before the procedure. Antiseptics must not be used for speculum treatment. The sample must be taken from the lateral or posterolateral vaginal wall.

From virginal women, sample must be taken from the entrance of vagina, or in special cases from the posterior vaginal wall through the hymenal rings.

The features of the urethral sampling:

Patient must not urinate within 1.5-2 hours prior to sampling procedure.

The external urethral orifice must be treated with a swab moistened with sterile physiological saline solution just prior to the sampling procedure.

In the case of purulent discharge, the sample must be taken 15-20 minutes after urinating. In the absence of discharge, it is necessary to massage urethra with sampling swab or brush.

Carefully insert the swab into the woman’s urethra to a depth of 1.0-1.5 cm. A child’s sample must be taken from the external urethral orifice.

The features of the cervical sampling:

Remove mucus with a cotton swab prior to sampling, and treat the cervix with sterile physiological saline solution.

Carefully insert sampling swab into the cervix to a depth of 0.5-1.5 cm.

Avoid contact with vaginal wall when removing the swab.

Order of taking:

1. Open the tube.

2. Scrape epithelial cells from the corresponding biotope (i.e., vagina, urethra, cervix) with a sterile swab.

3. Put the swab into the tube with transport medium and rinse it thoroughly. Avoid spraying of solution.

4. Remove the swab from solution, press it to the wall of tube and squeeze the rest of the liquid. Throw out the swab. Use a new swab if you need to repeat sampling or to take sample from another biotope.

5. Close the tube tightly and mark it.

Transportation and storage of the samples

Overall time from the sample intake until analysis must not exceed 24 hours.

Samples may be transported and stored in physiological saline at temperatures from 2 °C to 8 °C no more than 24 hours prior to analysis. When it is impossible to deliver the material in the laboratory during the day, a one-time freezing of the material is allowed. The frozen material is allowed to be stored at temperatures from minus 18 °C to minus 22 °C for one month.

In case of usage transport media biological material samples are transported and stored according to the instruction for the transport medium used intended for subsequent sample analysis by PCR.

The detailed description of sampling and sample processing procedures as well as sample storage and transportation requirements cited in **PREP-NA PLUS**, **PREP-GS PLUS** and **PREP-MB RAPID** extraction kits user manuals.

8. PROCEDURE

DNA extracting from biological material

DNA extraction is carried out according to the extraction kit instructions. **PREP-NA PLUS**, **PREP-GS PLUS** and **PREP-MB RAPID Extraction Kit** are recommended.

A DNA extraction kit is not included in **Femoflor® 16 REAL-TIME PCR Detection Kit**.

If the sample is taken in a tube with sterile physiological saline solution, the "DNA Technology" made **PREP-NA PLUS**, **PREP-GS PLUS** or **PREP-MB RAPID** extraction kits are recommended for DNA extraction. If the sample is taken in a tube with the "PREP-RAPID" reagent, **PREP-NA PLUS DNA/RNA Extraction Kit** is recommended for DNA extraction.

Enquire with customer service about compatibility of third-party DNA extraction kits with **Femoflor® 16 REAL-TIME PCR Detection Kit.**

Independently of DNA extraction kit used, a negative control sample should go through all stages of DNA extraction. Physiological saline solution can be used as a negative control sample with its volume according DNA extraction kit used.

Assay procedure

The reagents and tubes should be kept away from direct sunlight.

Strictly observe the completeness of the strips and caps for them. Do not use the caps for the strips of the other kits!

8.1 Mark the required number of strips with paraffin sealed PCR-mix for each test sample, positive control (C+) and negative control (C-).

Two strips are designed for one sample assay.

Example: to test 2 samples, mark 8 strips - 4 strips for the samples, 2 strips for "C-" and 2 strips for "C+". See Table 3 for reference.

Table 3. Tube marking

	Femoflor® 16 REAL-TIME PCR Detection Kit
Sample 1	Tubes 1-8 (strip-1 and strip-2)
Sample 2	Tubes 1-8 (strip-1 and strip-2)
C+	Tubes 1-8 (strip-1 and strip-2)
C-	Tubes 1-8 (strip-1 and strip-2)

8.2 Vortex the Taq-polymerase solution for 3-5 seconds, then spin for 1-3 seconds.

8.3 Add 10 µL of Taq-polymerase solution into each tube. Avoid paraffin layer break.

8.4 Add one drop (~20 µL) of mineral oil into each tube of the strip.

8.5 Vortex the tubes with samples, "C+" and "C-" and for 3-5 seconds and spin down drops for 1-3 seconds.

In case of using **PREP-GS PLUS DNA Extraction Kit**. After vortexing centrifuge the tubes with the DNA preparation at RCF(g) 16000 for one minute to precipitate the sorbent. If, after isolation, the supernatant containing the isolated DNA was transferred to new tubes, centrifugation is carried out for 1-3 seconds in a vortex mixer.

When using the **PREP-MB RAPID DNA Extraction Kit** for DNA extraction, it is necessary to place the tubes with the DNA preparation into a magnetic tube rack after vortex. If, after extraction, the supernatant containing the extracted DNA was transferred into new test tubes, centrifugation after vortex is performed in vortex-mixer for 3-5 seconds.

Open the strip, add DNA sample (or control sample), then close the strip before proceeding to the next strip to prevent contamination. Use filter tips. Close the strips tightly.

8.6 Add 5.0 µL of DNA sample into corresponding strips. Do not add DNA into the “C+”, “C-” strips. Avoid paraffin layer break.

8.7 Add 5.0 µL of negative control (C-) which passed whole DNA extraction procedure into corresponding strip. Add 5.0 µL of positive control sample (C+) into corresponding strip. Avoid paraffin layer break.

8.8 Spin strips for 3-5 seconds.

8.9 Set the strips into the Real-time Thermal Cycler.

8.10 Launch the operating software for DT instrument[1]. Add corresponding test[2], specify the number and ID’s of the samples, positive and negative control samples. Specify the position of the strips in the thermal unit (see 8.9) and run PCR. See Table 4.

Table 4. The PCR program for DTlite and DTprime Thermal Cyclers

Step	Temperature, °C	Min.	Sec.	Number of cycles	Optical measurement	Type of the step
1	80	0	30	1		Cycle
	94	1	30			
2	94	0	30	5		Cycle
	64	0	15		v	
3	94	0	10	45		Cycle
	64	0	15		v	
4	94	0	5	1		Cycle
5	10	…	…	Holding		Holding

[1] Please, apply to Operation Manual for DTprime and DTlite Real-Time PCR instruments PART II.
[2] Instructions for uploading "files with test parameters" can be found on "DNA-Technology's" website https://www.dna-technology.com/assaylibrary.

9. CONTROLS

The **Femoflor® 16 REAL-TIME PCR Detection Kit** contains positive control sample. Positive control is a cloned part of the specific genome. It is produced with genetic engineering techniques and characterized by automatic DNA sequencing. The PCR-mix from the kit includes the internal control (IC). IC is an artificial plasmid intended to assess the quality of PCR performance. The PCR-mix contains sample intake control (SIC). Sample intake control (SIC) estimates the amount of human DNA in the tube. To reveal possible contamination a negative control is required.

A negative control sample should go through all stages of DNA extraction. Physiological saline solution can be used as a negative control sample in volumes indicated in supplied instructions.

The test result is considered invalid when the exponential growth of the fluorescence level for the specific product and for internal control (IC) are not observed.

SIC value must be considered when analyzing results: SIC values lower than 4.0 should be considered as an insufficient amount of sample, and the sampling procedure must be repeated.

The test result is considered valid when:

In positive control sample positive result must be determined: decimal logarithm of concentration or “+”. In case of negative values (“-”) the results of the current batch are considered false. In this case it is required to repeat amplification of all samples.

In negative control sample negative result must be determined (“-”) for specific target and positive result for internal control. In case of different values the results of the current batch are considered false. In this case conduction of decontamination procedures is required.

10. DATA ANALYSIS

Registration and interpretation of the PCR results are held in automatic mode. The identificator of sample, test name and result for each target (quantity and diagram allowing a relative comparison of normal flora and opportunistic pathogens in each sample) will be displayed in the right module of the window. A qualitative analysis will be performed for pathogens. The resulting graph will display the dependence of fluorescence intensity on cycle number for each tube.

To create a Specific report for Biocenose press the “Form the answer button”.

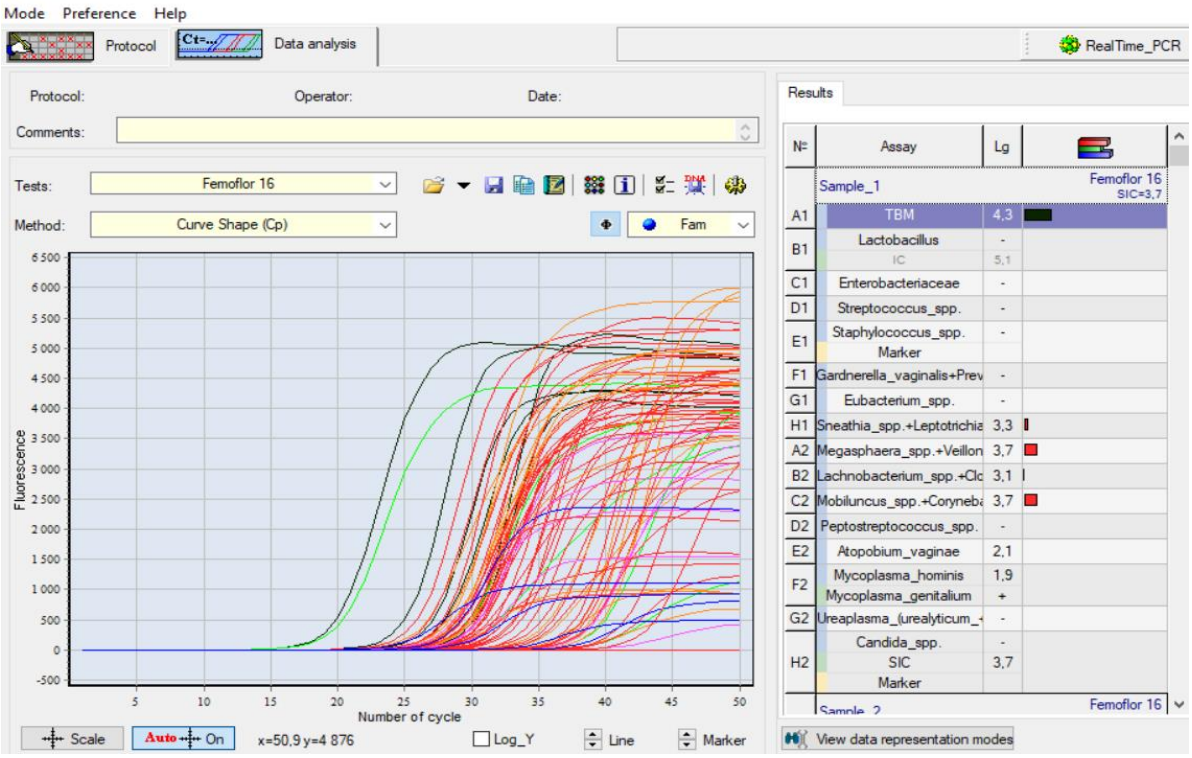

Urogenital microbiome composition test
Femoflor 16

Logotype

Date
Number of tube
Patient name
Sex
Age
Organization
Clinician name
Comments

Information about laboratory

Sample ID: C+

№	Test title	Result	
		Quantitative	Relative Lg(X/TMD)
	Sample intake control	$10^{4.7}$ ☐	
1	Total Bacterial Mass	$10^{7.4}$ ☐	
	Normal microflora		
2	Lactobacillus	$10^{7.4}$	0.0 (82-100%) ■
	Facultative anaerobic microorganisms		
3	Enterobacteriaceae	not detected	☐
4	Streptococcus spp.	$10^{5.6}$	-1.8 (1.3-1.8%) ☐
5	Staphylococcus spp.	$10^{4.5}$	-2.9 (0.1-0.1%) ☐
	Obligate anaerobic microorganisms		
6	Gardnerella vaginalis+Prevotella bivia+Porphyromonas spp.	$10^{4.3}$	-3.1 (<0.1%) ☐
7	Eubacterium spp.	$10^{5.0}$	-2.4 (0.3-0.4%) ☐
8	Sneathia spp.+Leptotrichia spp.+Fusobacterium spp.	not detected	☐
9	Megasphaera spp.+Veillonella spp.+Dialister spp.	$10^{3.5}$	-3.9 (<0.1%) ☐
10	Lachnobacterium spp.+Clostridium spp.	$10^{4.3}$	-3.1 (<0.1%) ☐
11	Mobiluncus spp.+Corynebacterium spp.	$10^{5.6}$	-1.8 (1.3-1.8%) ☐
12	Peptostreptococcus spp.	$10^{4.2}$	-3.2 (<0.1%) ☐
13	Atopobium vaginae	not detected	☐
	Yeast-like fungi		
14	Candida spp. *	$10^{3.4}$ ☐	
	Mycoplasmas		
15	Mycoplasma hominis *	not detected ☐	
16	Ureaplasma (urealyticum + parvum) *	not detected ☐	
	Pathogenic microorganisms		
17	Mycoplasma genitalium **	not detected ☐	

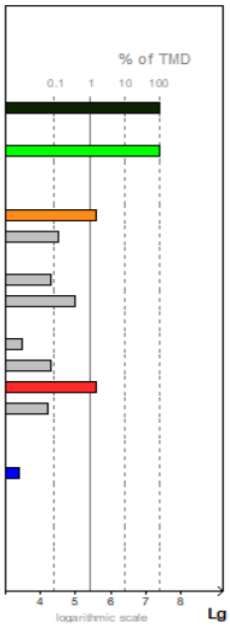

* Quantitative Analysis Lg(X) ** Qualitative Analysis *** Below threshold

Conclusion:
Absolute normocenosis

In case of using DNA-Technology made Real-Time PCR Thermal Cyclers, the analysis is performed automatically.

The quantitative measure (logarithm of concentration) and diagram are displayed in the line with taxonomic identifier of bacteria detected by **Femoflor® 16 REAL-TIME PCR Detection Kit**.

In the samples free of specific product DNA, the Real-time PCR thermal cycler registers the expressed growing fluorescence of the internal control and its absence for the specific product.

In the absence of specific signal and IC signal the program registers unreliable result. It is necessary to repeat the analysis for the given sample. An unreliable result may be due to the presence of inhibitors in the DNA preparation; incorrect implementation of the analysis protocol, violation of the amplification temperature regime, etc. In this case, it is necessary to repeat PCR amplification, or DNA isolation and PCR, or sampling procedure for the given patient (performed sequentially).

When SIC value is lower than 4.0, it should be considered as insufficient amount of human DNA in sample and the sampling procedure must be repeated.

For positive control samples, the program registers a positive result. When negative results are obtained, all results of corresponding experiment should be considered as false. All samples must be reanalyzed.

For negative control samples, the program registers a negative result. When positive results are obtained, all results of the corresponding experiment should be considered as false and the PCR laboratory must be decontaminated.

11. SPECIFICATIONS

a. The specificity of the **Femoflor® 16 REAL-TIME PCR Detection Kit** was assessed by bioinformatics analysis using available on-line databases with up-to-date comprehensive genetic information. The specific oligonucleotides used in the test were checked against GenBank database sequences. None of the sequences showed sufficient similarity for unspecific detection.

The samples with specific product DNA are to be registered positive for specific product (a fragment of the specific product genome). The samples free of specific product DNA are to be registered negative for specific product and positive for internal control.

The lists of microorganisms identified by the kit are presented in Table 5.

Table 5. The list of microorganisms identified by the **Femoflor® 16 REAL-TIME PCR Detection Kit**.

№ of tube in a strip	Dye label/detection channel		
	Fam	**Hex**	**Rox**
Strip-1			
1	Total bacterial mass (TBM)	-	-
2	*Lactobacillus* spp.	IC	-
3	*Enterobacteriaceae*	-	-
4	*Streptococcus* spp.	-	-
5	*Staphylococcus* spp.	-	Marker
6	*Gardnerella vaginalis*/*Prevotella bivia*/ *Porphyromonas* spp.	-	-
7	*Eubacterium* spp.	-	-
8	*Sneathia* spp./*Leptotrihia* spp./ *Fusobacterium* spp.	-	-
Strip-2			
1	*Megasphaera* spp./*Veilonella* spp./ *Dialister* spp.	-	-
2	*Lachnobacterium* spp./*Clostridium* spp.	-	-
3	*Mobiluncus* spp./*Corynebacterium* spp.	-	-
4	*Peptostreptococcus spp.*	-	-
5	*Atopobium vaginae*	-	-
6	*Mycoplasma hominis*	*Mycoplasma genitalium*	-
7	*Ureaplasma (urealyticum + parvum)*	-	-
8	*Candida* spp.	SIC	Marker

b. In a determination of analytical sensitivity, the **Femoflor® 16 REAL-TIME PCR Detection Kit** demonstrated the ability to reproducibly detect 5 or more copies of purified pathogens DNA per PCR reaction. The copy number of the pathogens was determined by Poisson analysis.

The **Femoflor® 16 REAL-TIME PCR Detection Kit** detects one CFU of the pathogen per PCR reaction. This analytical sensitivity was determined by serially diluting pathogens infected cultures in culture transport media. Samples of each dilution were processed and tested by the standard Kit procedure. Each of the replicates containing 1 CFU per amplification reaction gave a strong positive signal.

Analytical sensitivity is no more than 10000 copies/mL.

c. Diagnostic characteristics

Diagnostic sensitivity: 97%.

Diagnostic specificity: 97%.

The claimed specifications are guaranteed when DNA extraction is performed with **PREP-NA PLUS** REF P-002/1EU, **PREP-GS PLUS** REF P-003/1EU and **PREP-MB RAPID** (REF P-116-A/8EU) extraction kits.

12. TROUBLESHOOTING

Table 6. Troubleshooting

	Result	Possible cause	Solution
C+	-	Operation error PCR inhibition Violation of storage and handling requirements	Repeat whole test Dispose current batch
C-	+	Contamination	Dispose current batch Perform decontamination procedures
IC	Invalid	PCR inhibition	Repeat whole test Resample

If you face to any undescribed issues contact our customer service department regarding quality issues with the kit:

Phone: +7(495)640.16.93

E-mail: hotline@dna-technology.ru

https://dna-technology.com/support.

13. QUALITY CONTROL

"DNA-Technology Research&Production", LLC declares that the above mentioned products meet the provision of the Council Directive 98/79/EC for *in vitro* Diagnostic Medical Devices. The quality control procedures performed in accordance with ISO 9001:2015 and ISO 13485:2016:

- observation of quality management in manufacturing of IVDD products;
- creation of values for customers;
- maintenance of the best service quality and customer management.

Contact our official representative in EU by quality issues of **Femoflor® 16 REAL-TIME PCR Detection Kit**.

Technical support:

E-mail: hotline@dna-technology.ru

https://www.dna-technology.com

Manufacturer: "DNA-Technology Research & Production", LLC,

142281, Russia, Moscow Region,

Protvino, Zheleznodorozhnaya Street, 20

Phone/fax: +7(495) 640.17.71

E-mail: info@dna-technology.com

https://www.dna-technology.com

Authorized representative in EU:

OBELIS S.A

Registered Address:

Bd. Général Wahis, 53

1030 Brussels, Belgium

Tel: +32.2.732.59.54

Fax: +32.2.732.60.03

E-mail: mail@obelis.net

http://www.obelis.net

14. KEY TO SYMBOLS

IVD	*In vitro* diagnostic medical device		Date of manufacture
	Temperature limit		Consult instructions for use
	Contains sufficient for <n> tests	REF	Catalogue number
	Use-by date		Manufacturer
LOT	Batch code		Keep away from sunlight
	Caution	VER	Version
CONTROL +	Positive control	NON STERILE	Non-sterile
EC REP	Authorized representative in the European Community		Do not reuse

REF R1-P801-S3/6EU

VER 513-3.2022.08.25